

BEGO IMPLANT SYSTEMS PRODUCT CATALOGUE

2017/2018

Partners in Progress



The Evolution of the BEGO Semados® S-Line



BEGO SEMADOS® S IMPLANTS HAVE BECOME SC AND SCX IMPLANTS.*

www.bego.com/scx



*For more information on our new products and their availability, please visit www.bego.com/scx

GENERAL	5
Foreword	5
BEGO – Solutions from a single source	6
REGENERATION	9
BEGO Biomaterials	10
SURGERY	11
Descriptions and labelling	12
Implant planning aids	15
SC/SCX Implants with PS* ⁵ design	17
RS/RSX Implants with PS* ⁵ design	21
RI Implants with PS* ⁵ design	25
Cover Screws / Healing Posts with PS* ⁵ design	27
Mini-implants / Healing Posts	31
Provisional Implant System	33
BEGO GUIDE GUIDED SURGERY	37
Preparation Instruments	45
Bone Shapers / Trepanns	56
Surgical Instruments	57
Cover Screws / Healing Posts without PS* ⁵ design	99
PROSTHETICS	59
Prosthetic Instruments	60
CAD / CAM Implant Prosthetics Bego Medical	61
• Interface summary	62
• BEGO CADAbut F –one-part individual healing posts	62
• BEGO CADAbut F –two-part individual healing posts	62
• BEGO CADAbut F –one-part individual abutments	63
• BEGO CADAbut F –two-part individual abutments	63
• BEGO CADBase (bar bases)	64
• BEGO CADBar	64
• Additional holding elements	65
• Bar secondary structure	65
• Bridge bases	66
• Zirconia Maryland bridges	66
SC/SCX/RS/RSX/RI*¹ prostheses with PS*⁵ design	67
• CAD/CAM restoration	68
• One Care Package restoration	71
• Impression taking and model fabrication	72
• Crown restoration Ø3.0	73
• Crown and bridge restoration	74
• Multi ⁱ Plus restoration	80
• Hybrid restoration	85
• Screws	89
Mini-Line prostheses	91
• CAD/CAM restoration	92
• Impression taking and model fabrication	92
• Crown restoration	93
• Hybrid restoration	94
• Screws	97
S/RI prostheses without PS*⁵ design	101
• CAD/CAM restoration	102
• Impression taking and model fabrication	104
• Crown and bridge restoration	105
• Multi ⁱ Plus restoration	110
• Hybrid restoration	115
• Screws	118

*⁵ Platform Switch Design

DEMO MODELS / MATERIAL **119**

Large-scale models	120
Demonstration material	121

SERVICE **123**

Torque specifications	124
Material specifications	126
Index by article numbers	130
Alphabetical index	144

Note: Depending on regulatory approvals, under some circumstances not all offered products or services will be available worldwide.
Please contact your local BEGO Implant Systems sales partner.

Images and illustrations are examples only and the colours, symbols, design and specifications on the labels and/or packages shown may deviate from real products.

Specifications for lengths and diameters may be rounded up or down for simplification.

Our products are constantly being refined. We therefore reserve the right to make changes.

© 2017 by BEGO Implant Systems GmbH & Co. KG, Bremen. We reserve all rights to reprints of extracts, photomechanical reproduction and particularly translations.

Durable, lasting value and sustainable – all on the safe side



Walter Esinger
Managing Director at BEGO Implant Systems

Dear customers and partners

Digitalisation and patient-specific restorations are the measure of all things in implant dentistry. The digital value creation process from implantation using surgical guides through intraoral impression taking to treating the patient with customised prosthetic solutions is increasingly the standard in modern implant dentistry.

In this situation, it is more important than ever before to know that you have a reliable partner at your side, one with the necessary expertise based on long experience – BEGO Implant Systems.

Our daily actions demonstrate our commitment to our social responsibility as a medium-sized employer in the Bremen region. Our products are particularly needs oriented, durable, stable in value and sustainable. We are guided by the values of trust and reliability and they form the basis of our collaborations with our customers and partners and our employees.

Our vision: 'In all mouths and around the world: We would like specifically to become a nationally and internationally valued, strong growing and sustainable brand.'

Our common goal: Premium customer services and strengthening economic cohesion to ensure healthy growth. This is what BEGO Implant Systems stands for. With us, you are on the safe side and ahead of the rest.

In short, we offer holistic implant dentistry system solutions from Germany – and service that leaves dentists and patients around the world smiling with satisfaction: on a partnership, personal and professional level.

Bremen, Spring 2017

Walter Esinger


Solutions from a single source



Conventional solutions

BEGO Bremer Goldschlägerei GmbH & Co. KG develops and sells precious metal and non-precious metal dental alloys and provides equipment, materials and services for fabricating premium dental restorations. The company also offers ceramics for further processing in the dental laboratory.

Since its founding and now moving into its fifth generation, BEGO has put into practice its aim of providing dental laboratories with innovative and cost-effective products and services for optimal treatment of their patients, all from a single source.

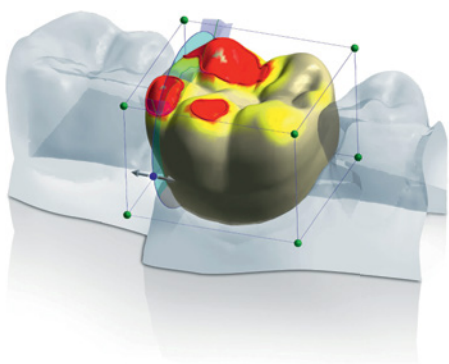

CAD / CAM solutions

BEGO Medical GmbH specialises in digital processes and is a pioneer in CAD / CAM technology in the dental sector. The company is the inventor and holder of the patent for the Selective Laser Melting (SLM) procedure in the dental sector. All-round expertise in procedures and the widest choice of materials mean our customers have access to premium quality products and services across a large number of indications. In its high-tech production centre located in Bremen, BEGO fabricates frameworks, abutments, crowns and bridges based on virtual models using the latest laser and milling techniques in four different procedures: SLM, High Speed Cutting (HSC), CAD/Cast® and Rapid Prototyping.



Implant dentistry solutions

Since 1990 BEGO Implant Systems GmbH & Co. KG has been developing and fabricating dental implants and supplementary products to treat patients with implants throughout the world. An innovative 3D implant design, system abutments for modern implant dentistry, a safe biomaterials system and functionally optimised guided surgery all mean that dental implants 'Made by BEGO' lead to planned and reproducible results. These are premium German products that incorporate technological advances at a fair price, combining safety, durability, aesthetics and reliability.



BEGO TRAINING CENTER

Practical knowledge of subjects such as CAD / CAM or traditional dental technology are taught by an internationally experienced team of trainers in courses – both for beginners and advanced users – specifically tailored to meet the most diverse requirements.

Our in-house course concepts form the basis of a challenging program for seminars and practical courses that help interested dental technicians to become even more successful.

Professional development: A focus of BEGO Implant Systems

BEGO Academia Implantology

Supporting postgraduate dental training and qualification of dental technicians in the area of modern, implant-retained prosthetics is the focus of BEGO Implant Systems – and has been right from the start.

So that we can continuously optimise our training programs, we have formed a number of framework agreements with national and international professional development training centres under the umbrella trademark 'BEGO Academia Implantology'. You can read about our national training programs in our course brochure. Visiting our website is another way to find out more about the latest courses on offer.

For international training programs, please contact our worldwide sales partners or contact BEGO Implant Systems in Bremen directly.

For professional development courses for dental technicians, the academia dental® (<http://www.academia-dental.de>) and the BEGO TRAINING CENTER (<http://www.bego.com/courses-events/education/bego-training-center/>) in Bremen are also available.

Is there a course or training program you'd like to see offered? We look forward to any suggestions you may have.









OVERVIEW

BEGO Biomaterials

10

Biomaterials					
Description	REF	Size		Contents	
BEGO OSS Bovine Bone Graft Substitute	57212	Particle size	0.5–1 mm	0.5 mL	
	57213	Particle size	0.5–1 mm	1 mL	
	57214	Particle size	0.5–1 mm	3 mL	
	57215	Particle size	1–2 mm	2 mL	
	57216	Particle size	1–2 mm	5 mL	
BEGO OSS S Synthetic Bone Graft Substitute	57217	Particle size	0.5–1 mm	0.5 mL	
	57218	Particle size	0.5–1 mm	1 mL	
	57219	Particle size	0.8–1.5 mm	2 mL	
BEGO Collagen Fleece Short-term Regeneration Matrix	57220	20 × 20 mm		12 units	
BEGO Collagen Membrane Barrier Membrane Derived from porcine pericardium	57221	15 × 20 mm		1 unit	
	57222	20 × 30 mm		1 unit	
	57223	30 × 40 mm		1 unit	


Note: Depending on regulatory approvals, under some circumstances not all products in the BEGO Biomaterials Systems will be available worldwide. Please contact your local BEGO Implant Systems sales partner.



OVERVIEW

Descriptions and labelling	12
Implant planning aids	15
BEGO Semados® SC/SCX Implants with Platform Switch Design	17
BEGO Semados® RS/RSX Implants with Platform Switch Design	21
BEGO Semados® RI Implants with Platform Switch Design	25
Cover screws / healing posts with Platform Switch Design	27
BEGO Semados® Mini Implants/healing posts	31
BEGO Semados® Provisional Implant System	33
BEGO GUIDE GUIDED SURGERY	37
Preparation instruments	45
Bone shapers/trepans	56
Surgical instruments	57
Cover screws / healing posts without Platform Switch Design	99

The evolution of the BEGO Semados® S-Line

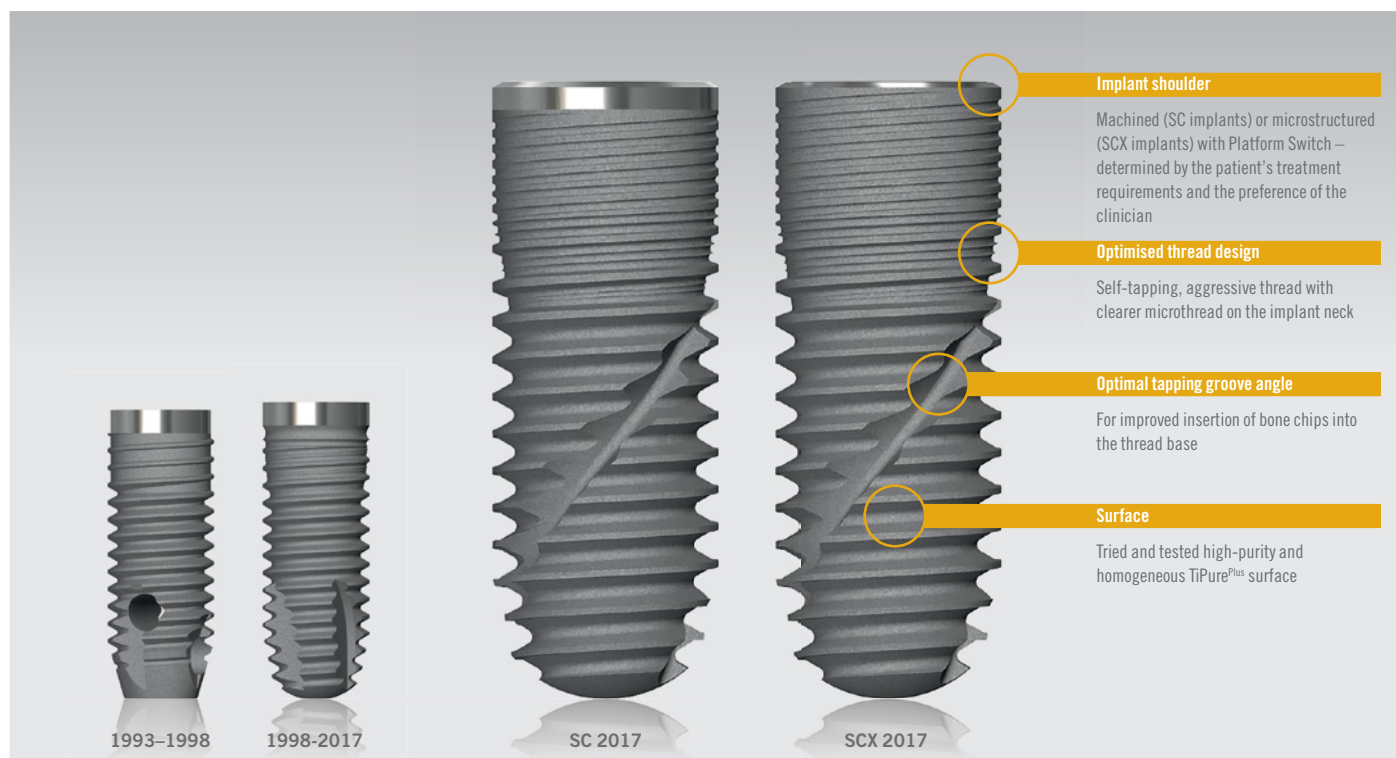

BEGO SEMADOS® S IMPLANTS ARE NOW SC AND SCX IMPLANTS.

Your established system with an improved design

The SC and SCX implants are the latest refinement of and replacement for the BEGO Semados® S implants. Both the SC and the SCX implant, along with the S implants, will be prepared with the existing BEGO Semados® S-Line Tray^{Plus}.















The new systems have an indentation on the implant shoulder (the Platform Switch) which means that S-Line customers can benefit from Platform Switch prosthetics (PS-Line) using the new implants. Individual restorations made from a wide variety of materials can be fabricated as usual using the CAD / CAM system from BEGO Medical GmbH. The tried and true conical inner connection with a mean conical angle of 45° and the internal hex that acts as an anti-rotation mechanism mean that the new SC and SCX implants are compatible with existing prostheses in the RS / RSX-Line. Users can still access all the usual Platform Switch prosthetic components.

The new implants are available in the familiar diameters and lengths of the S-Line and are suitable for almost every indication in implant dentistry. An implant with a diameter of 5.5 and a length of 7 mm has been added to the range to satisfy customer requests for short and large-diameter implants.












The BEGO Semados® implant family


SC implant Self-tapping, cylindrical implant with 0.5 mm machined implant shoulder
SCX implant Self-tapping, cylindrical implant with 0.1 mm machined implant shoulder
RS implant Self-tapping, conical implant with 0.5 mm machined implant shoulder
RSX implant Self-tapping, conical implant with 0.1 mm machined implant shoulder
RI implant – NEW – with Platform Switch Self-condensing, conical implant with 0.5 mm machined implant shoulder
Mini implant Reduced diameter, condensing, conical implant with 0.8 mm machined implant shoulder


Colour coding / diameter

BEGO Semados® RS/RSX implant 3.0	  Ø 3.0 mm
BEGO Semados® Mini implant 2.7/2.9/3.1	  Ø 3.5 mm
BEGO Semados® S/ SC / SCX implant 3.25	  Ø 3.67 mm
BEGO Semados® S/SC/SCX/RS/RSX/RI implant 3.75	  Ø 3.67 mm
BEGO Semados® S/SC/SCX/RS/RSX/RI implant 4.1	  Ø 4.1 mm
BEGO Semados® S/SC/SCX/RS/RSX/RI implant 4.5	  Ø 4.5 mm
BEGO Semados® S/SC/SCX/RS/RSX/RI implant 5.5	  Ø 5.5 mm

Colour coding / diameter

1		Manufacturer
2		Article name / Size specification
3	<div> <div> <div></div> <div>Ø 3.0</div> </div> <div> <div></div> <div>Ø 2.7/2.9/3.1</div> </div> <div> <div></div> <div>Ø 3.25</div> </div> <div> <div></div> <div>Ø 3.75</div> </div> <div> <div></div> <div>Ø 4.1</div> </div> <div> <div></div> <div>Ø 4.5</div> </div> <div> <div></div> <div>Ø 5.5</div> </div> </div>	Colour coding
4	<div>REF</div> <div>LOT</div> <div></div>	Article number Batch code Use by
5	<div>CE</div> <div></div> <div>STERILE R</div> <div></div> <div></div> <div></div> <div></div> <div></div> <div></div> <div></div>	CE mark Do not reuse Sterilized using irradiation Do not resterilise Non-sterile Consult instructions for use Do not use if packaging is damaged Caution Temperature limit Do not expose to direct sunlight RxOnly Federal law (USA) restricts this product to sale by or on the order of a dentist or physician in the USA.  Speed
6		DataMatrix code Contains the manufacturer name and article number. If applicable, the batch code and/or expiry date as well
7		Sticker for documentation purposes

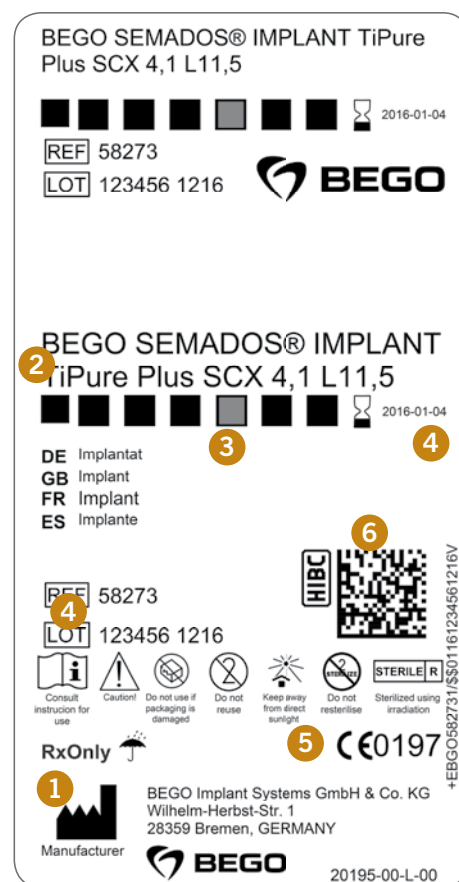

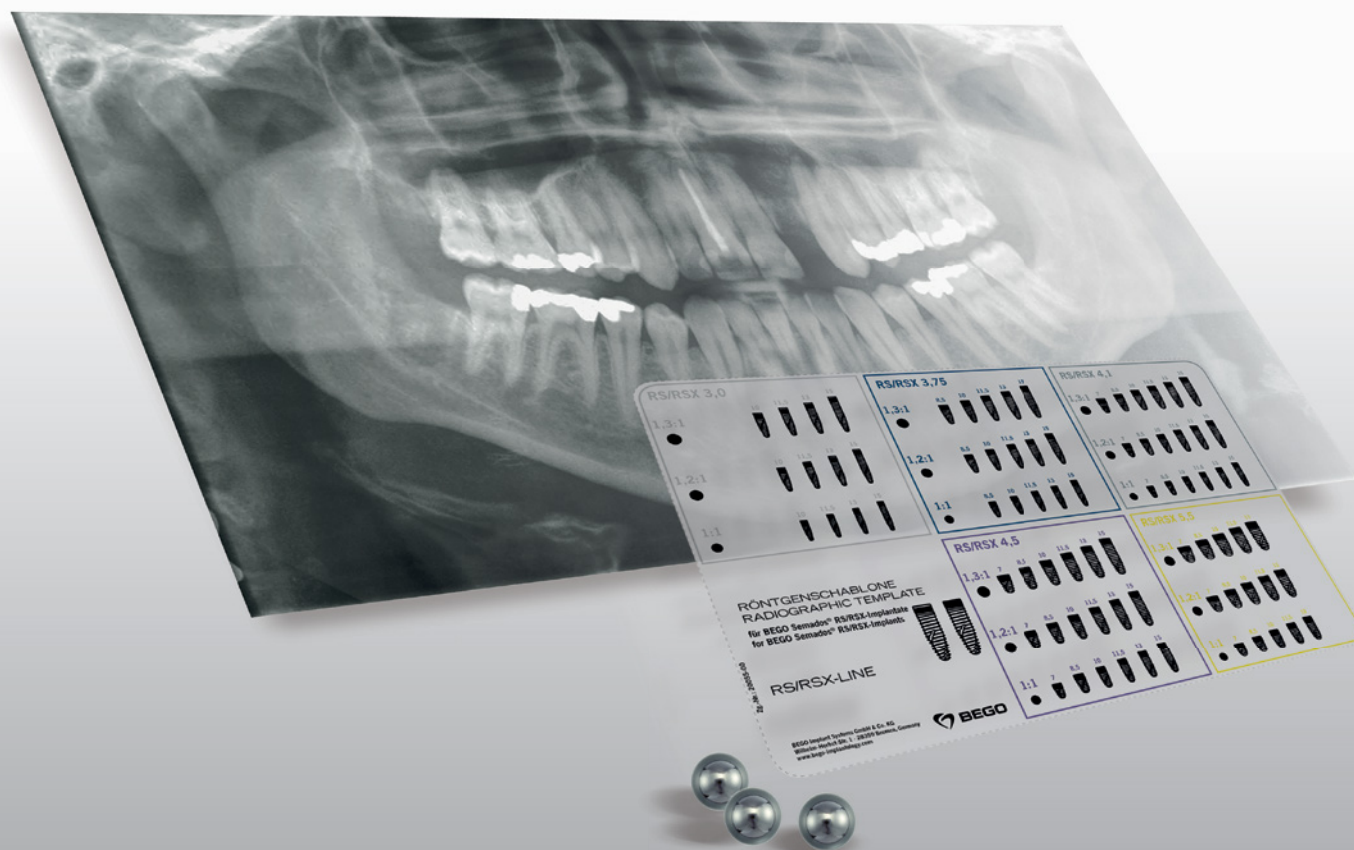


OVERVIEW

Implant planning aids

16

Implant planning aids					
Description	REF	Colour code	Size	Compatibility	Units
Measuring spheres for the radiograph template	53889		Ø 4 mm		10
Radiograph templates	53888			S implants	1
	58246			SC/SCX implants	1
	57959			RS/RSX implants	1
	55745			RI implants	1
	57010			Mini implants	1
	57672			PI implants	1
Drill sleeves for preparing customised drilling templates	55512		Fits in REF 55513	Pilot drill / pilot marker Ø 1.6 mm	4
	55513			Depth drill Ø 2.5 mm	4
	57596		Fits in REF 57597	Pilot drill / pilot marker Ø 2.5 mm	4
	57597			Depth drill Ø 3.2 mm	4



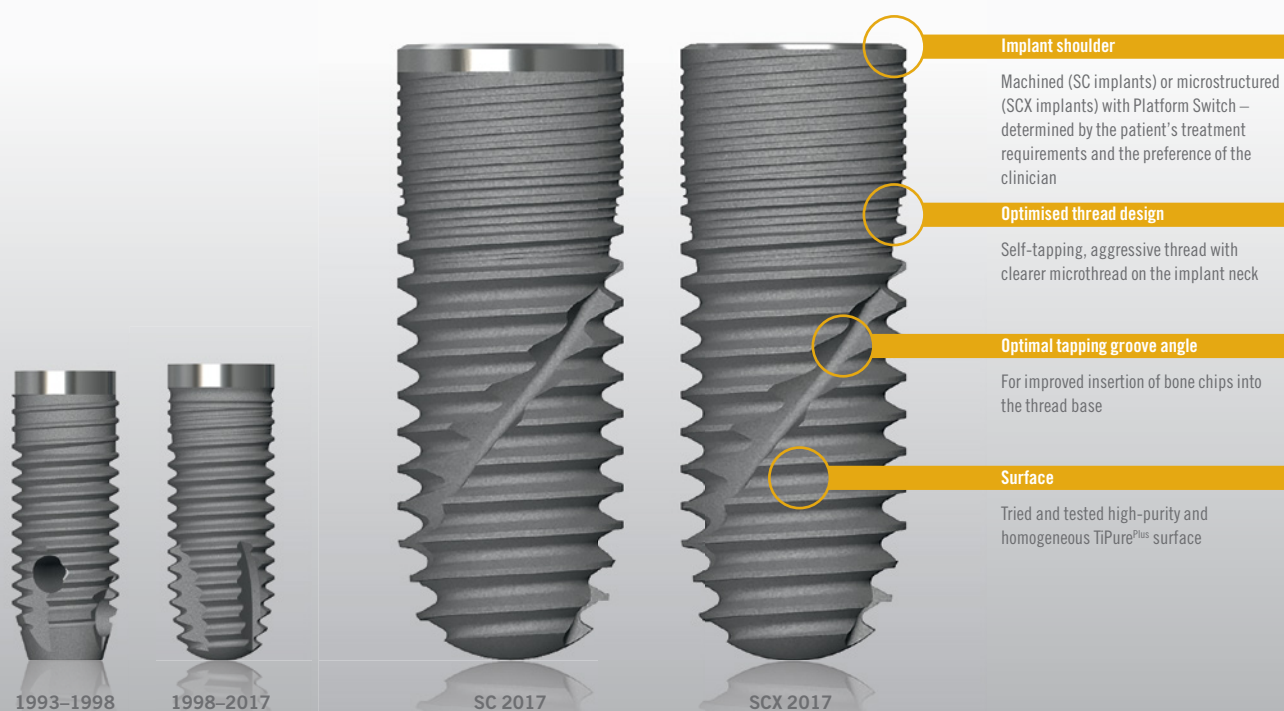

BEGO SEMADOS® S IMPLANTS ARE NOW SC AND SCX IMPLANTS.

Your established system with an improved design

The BEGO Semados® SC/SCX implant is a self-tapping, cylindrical implant made of pure titanium (grade 4). In contrast to the SCX implant, the SC implant has a machined neck region of 0.5 mm.






With an adequate bone level, it is recommended to use implants with a diameter $\geq \varnothing 4.5$ and for a low bone level a diameter ≤ 4.1 is recommended depending on the prosthetic concept. The reduced-diameter SC/SCX implant with a diameter of $\varnothing 3.25$ may only be used to restore narrow anterior gaps associated with the loss of teeth 12, 22, 33, 32, 31, 41, 42 and 43! Implant prosthetic concepts that exert a high mechanical force on the implants and the components (single crowns, double crowns, telescopic crowns, extension bars, etc.) should be implemented with large-diameter implants (> 4.0). For bar restorations, it is recommended to use a diameter ≥ 4.1 for the terminal implants.



Consult instructions for use

Recommended implant diameter (from the perspective of mechanical loading)								
Maxilla	3.25	–	+	–	–	–	–	–
	3.75	+	+	+	+	0	–	–
	4.1	+	+	+	+	+	+	+
	4.5	+	+	+	+	+	+	+
	5.5	+	+	+	+	+	+	+
Tooth / region	1	2	3	4	5	6	7	
Mandible	5.5	+	+	+	+	+	+	+
	4.5	+	+	+	+	+	+	+
	4.1	+	+	+	+	+	+	+
	3.75	+	+	+	+	0	–	–
	3.25	+	+	+	–	–	–	–

– = not suitable / 0 = suitable for reduced chewing force less than 150 N / + = suitable


Implants						
Description	REF	Colour code	Size	Compatibility	Units	
BEGO Semados® implants incl. cover screw and titanium insertion posts TiPure ^{plus} surface Material: Titanium grade 4 (packaged sterile)	58160	■	3.25 L8.5	SC	1	
	58161	■	3.25 L10	SC	1	
	58162	■	3.25 L11.5	SC	1	
	58163	■	3.25 L13	SC	1	
	58164	■	3.25 L15	SC	1	
	58165	■	3.75 L8.5	SC	1	
	58166	■	3.75 L10	SC	1	
	58167	■	3.75 L11.5	SC	1	
	58168	■	3.75 L13	SC	1	
	58169	■	3.75 L15	SC	1	
	58170	■	4.1 L7	SC	1	
	58171	■	4.1 L8.5	SC	1	
	58172	■	4.1 L10	SC	1	
	58173	■	4.1 L11.5	SC	1	
	58174	■	4.1 L13	SC	1	
	58175	■	4.1 L15	SC	1	
	58176	■	4.5 L7	SC	1	
	58177	■	4.5 L8.5	SC	1	
	58178	■	4.5 L10	SC	1	
	58179	■	4.5 L11.5	SC	1	
	58180	■	4.5 L13	SC	1	
	58181	■	4.5 L15	SC	1	
	58182	■	5.5 L7	SC	1	
	58183	■	5.5 L8.5	SC	1	
	58184	■	5.5 L10	SC	1	
	58185	■	5.5 L11.5	SC	1	
	58186	■	5.5 L13	SC	1	

Note: BEGO Semados® SC/SCX implants 3.25–4.5, template-guided preparation using the BEGO Guide System is an option.

*5 Platform Switch Design

Implants						
Description	REF	Colour code	Size		Compatibility	Units
BEGO Semados® implants incl. cover screw and titanium insertion posts TiPure ^{plus} surface Material: Titanium grade 4 (packaged sterile)	58260	■	3.25	L8.5	SCX	1
	58261	■	3.25	L10	SCX	1
	58262	■	3.25	L11.5	SCX	1
	58263	■	3.25	L13	SCX	1
	58264	■	3.25	L15	SCX	1
	58265	■	3.75	L8.5	SCX	1
	58266	■	3.75	L10	SCX	1
	58267	■	3.75	L11.5	SCX	1
	58268	■	3.75	L13	SCX	1
	58269	■	3.75	L15	SCX	1
	58270	■	4.1	L7	SCX	1
	58271	■	4.1	L8.5	SCX	1
	58272	■	4.1	L10	SCX	1
	58273	■	4.1	L11.5	SCX	1
	58274	■	4.1	L13	SCX	1
	58275	■	4.1	L15	SCX	1
	58276	■	4.5	L7	SCX	1
	58277	■	4.5	L8.5	SCX	1
	58278	■	4.5	L10	SCX	1
	58279	■	4.5	L11.5	SCX	1
	58280	■	4.5	L13	SCX	1
	58281	■	4.5	L15	SCX	1
	58282	■	5.5	L7	SCX	1
	58283	■	5.5	L8.5	SCX	1
	58284	■	5.5	L10	SCX	1
	58285	■	5.5	L11.5	SCX	1
	58286	■	5.5	L13	SCX	1



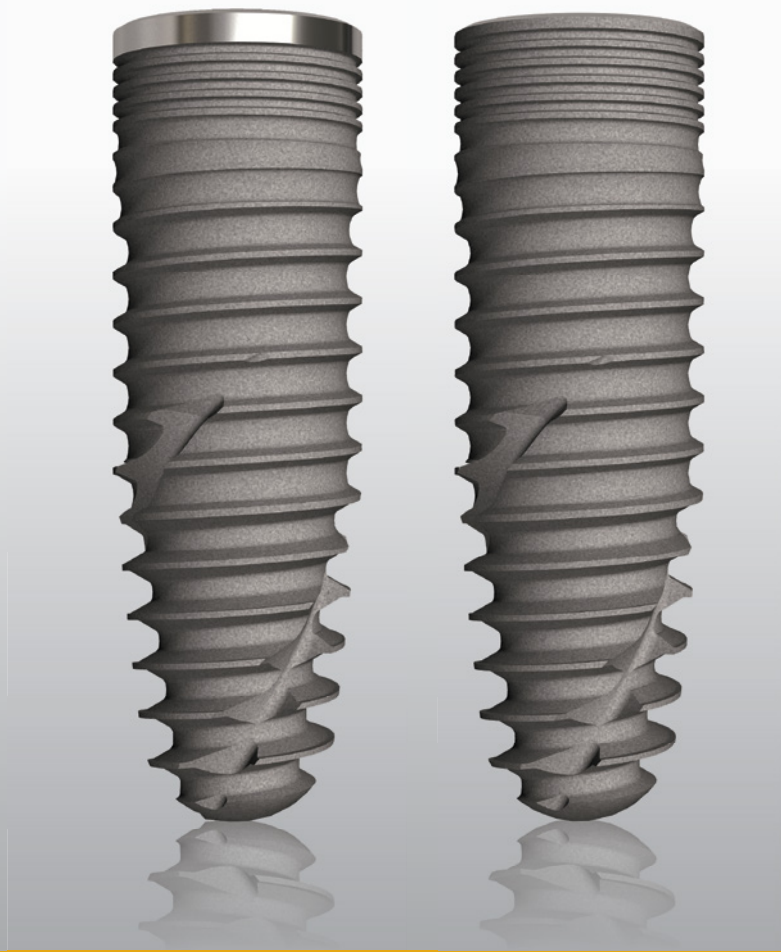

DESCRIPTION

The BEGO Semados® RS/RSX implant is a self-tapping, conical implant made of pure titanium (grade 4). In contrast to the RSX implant, the RS implant has a machined neck region of 0.5 mm.

If the bone level is sufficient, it is recommended to use the implant with the largest possible diameter depending on the prosthetic concept. The reduced-diameter RS/RSX implant with a diameter of 3.0 may only be used to restore narrow anterior gaps associated with the loss of teeth 12, 22, 32, 31, 41 and 42! Implant prosthetic concepts that exert a high mechanical force on the implants and the components should be implemented with large-diameter implants (> 4.0). For bar restorations, it is recommended to use a diameter ≥ 4.1 for the terminal implants.



Consult instructions for use

Recommended implant diameter
(from the perspective of mechanical loading)

Maxilla	3.0	–	+	–	–	–	–	–
	3.75	+	+	+	+	0	–	–
	4.1	+	+	+	+	+	+	+
	4.5	+	+	+	+	+	+	+
	5.5	+	+	+	+	+	+	+
Tooth / region		1	2	3	4	5	6	7
Mandible	5.5	+	+	+	+	+	+	+
	4.5	+	+	+	+	+	+	+
	4.1	+	+	+	+	+	+	+
	3.75	+	+	+	+	0	–	–
	3.0	+	+	–	–	–	–	–

– = not suitable / 0 = suitable for reduced chewing force less than 150 N / + = suitable

*5 Platform Switch Design

Implants						
Description	REF	Colour code	Size		Compatibility	Units
BEGO Semados® implants incl. cover screw and titanium insertion posts TiPure ^{plus} surface Material: Titanium grade 4 (packaged sterile)	57962	□	3.0	L10	RS	1
	57963	□	3.0	L11.5	RS	1
	57964	□	3.0	L13	RS	1
	57965	□	3.0	L15	RS	1
	57966	■	3.75	L8.5	RS	1
	57967	■	3.75	L10	RS	1
	57968	■	3.75	L11.5	RS	1
	57969	■	3.75	L13	RS	1
	57970	■	3.75	L15	RS	1
	57971	■	4.1	L7	RS	1
	57972	■	4.1	L8.5	RS	1
	57973	■	4.1	L10	RS	1
	57974	■	4.1	L11.5	RS	1
	57975	■	4.1	L13	RS	1
	57976	■	4.1	L15	RS	1
	57977	■	4.5	L7	RS	1
	57978	■	4.5	L8.5	RS	1
	57979	■	4.5	L10	RS	1
	57980	■	4.5	L11.5	RS	1
	57981	■	4.5	L13	RS	1
	57982	■	4.5	L15	RS	1
	57983	■	5.5	L7	RS	1
	57984	■	5.5	L8.5	RS	1
	57985	■	5.5	L10	RS	1
	57986	■	5.5	L11.5	RS	1
	57987	■	5.5	L13	RS	1



Note: BEGO Semados® RS /RSX implants 3.0–4.5, template-guided preparation using the BEGO Guide System is an option.

*5 Platform Switch Design

Implants						
Description	REF	Colour code	Size		Compatibility	Units
BEGO Semados® implants incl. cover screw and titanium insertion posts TiPure ^{plus} surface Material: Titanium grade 4 (packaged sterile)	57862	□	3.0	L10	RSX	1
	57863	□	3.0	L11.5	RSX	1
	57864	□	3.0	L13	RSX	1
	57865	□	3.0	L15	RSX	1
	57866	■	3.75	L8.5	RSX	1
	57867	■	3.75	L10	RSX	1
	57868	■	3.75	L11.5	RSX	1
	57869	■	3.75	L13	RSX	1
	57870	■	3.75	L15	RSX	1
	57871	■	4.1	L7	RSX	1
	57872	■	4.1	L8.5	RSX	1
	57873	■	4.1	L10	RSX	1
	57874	■	4.1	L11.5	RSX	1
	57875	■	4.1	L13	RSX	1
	57876	■	4.1	L15	RSX	1
	57877	■	4.5	L7	RSX	1
	57878	■	4.5	L8.5	RSX	1
	57879	■	4.5	L10	RSX	1
	57880	■	4.5	L11.5	RSX	1
	57881	■	4.5	L13	RSX	1
	57882	■	4.5	L15	RSX	1
	57883	■	5.5	L7	RSX	1
	57884	■	5.5	L8.5	RSX	1
	57885	■	5.5	L10	RSX	1
	57886	■	5.5	L11.5	RSX	1
	57887	■	5.5	L13	RSX	1



**Available from
March 2017**
with Platform Switch
Design



DESCRIPTION

The BEGO Semados® RI implant is a bone-condensing, non-self-tapping implant made of pure titanium (grade 4).

If the bone level is sufficient, it is recommended to use the implant with the largest possible diameter depending on the prosthetic concept. Implant prosthetic concepts that exert a high mechanical force on the implants and the components should be implemented with large-diameter implants (> 4.0). For bar restorations, it is recommended to use a diameter of 4.1 for the terminal implants.







Consult instructions for use

Recommended implant diameter (from the perspective of mechanical loading)								
Maxilla	3.75	+	+	+	+	0	–	–
	4.1	+	+	+	+	+	+	+
	4.5	+	+	+	+	+	+	+
	5.5	+	+	+	+	+	+	+
Tooth / region	1	2	3	4	5	6	7	
Mandible	5.5	+	+	+	+	+	+	+
	4.5	+	+	+	+	+	+	+
	4.1	+	+	+	+	+	+	+
	3.75	+	+	+	+	0	–	–


– = not suitable / 0 = suitable for reduced chewing force less than 150 N / + = suitable

*5 Platform Switch Design

Implants						
Description	REF	Colour code	Size	Compatibility	Units	
BEGO Semados® implants incl. cover screw and titanium insertion posts TiPure ^{plus} surface Material: Titanium grade 4 (packaged sterile)	57708	■	3.75 L8.5	RI*1	1	
	57709	■	3.75 L10	RI*1	1	
	57710	■	3.75 L11.5	RI*1	1	
	57711	■	3.75 L13	RI*1	1	
	57712	■	3.75 L15	RI*1	1	
	57718	■	4.1 L8.5	RI*1	1	
	57719	■	4.1 L10	RI*1	1	
	57720	■	4.1 L11.5	RI*1	1	
	57721	■	4.1 L13	RI*1	1	
	57722	■	4.1 L15	RI*1	1	
	57728	■	4.5 L8.5	RI*1	1	
	57729	■	4.5 L10	RI*1	1	
	57730	■	4.5 L11.5	RI*1	1	
	57731	■	4.5 L13	RI*1	1	
	57732	■	4.5 L15	RI*1	1	
	57738	■	5.5 L8.5	RI*1	1	
	57739	■	5.5 L10	RI*1	1	
	57740	■	5.5 L11.5	RI*1	1	
	57741	■	5.5 L13	RI*1	1	

*1 New version of the BEGO Semados® RI implants, with Platform Switch Design

*5 Platform Switch Design

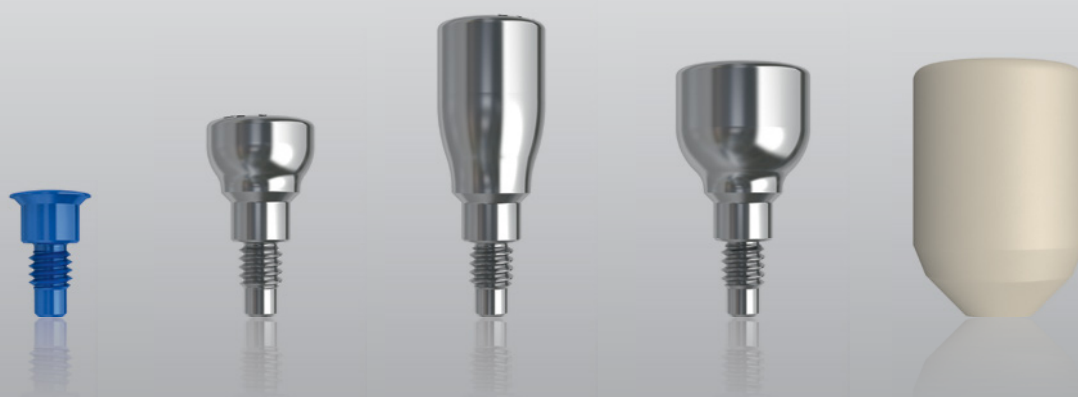

OVERVIEW

Cover screws Platform Switch
Healing posts Platform Switch

28

28

Cover screws Platform Switch

Description	REF	Colour code	Size	Compatibility	Units
Implant cover screw Material: Titanium grade 4 (packaged sterile) Tool: Hexagon screwdriver 1.25 mm *2	57950	□		RS/RSX 3.0	1
	58290	■		SC/SCX 3.25	1
	57951	■		SC/SCX/RS/RSX/RI*1 3.75	1
	57952	■		SC/SCX/RS/RSX/RI*1 4.1	1
	57953	■		SC/SCX/RS/RSX/RI*1 4.5	1
	57954	■		SC/SCX/RS/RSX/RI*1 5.5	1



Healing posts Platform Switch

Description	REF	Colour code	Size	Compatibility	Units
PS HP prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	Implant diameter 3.0				
	57764	□	Ø 3.0 L3	RS/RSX 3.0	1
	57765	□	Ø 3.0 L5	RS/RSX 3.0	1
	57766	□	Ø 3.0 L7	RS/RSX 3.0	1
	57767	□	Ø 4.0 L3	RS/RSX 3.0	1
	57768	□	Ø 4.0 L5	RS/RSX 3.0	1
	57769	□	Ø 4.0 L7	RS/RSX 3.0	1
	Implant diameter 3.25–3.75				
	57807	■	Ø 4.5 L3	SC/SCX/RS/RSX/RI*1 3.25–3.75	1
	57808	■	Ø 4.5 L5	SC/SCX/RS/RSX/RI*1 3.25–3.75	1
	58150	■	Ø 4.5 L7	SC/SCX/RS/RSX/RI*1 3.25–3.75	1
	Implant diameter 4.1				
	57809	■	Ø 5.0 L3	SC/SCX/RS/RSX/RI*1 4.1	1
	57810	■	Ø 5.0 L5	SC/SCX/RS/RSX/RI*1 4.1	1
	58151	■	Ø 5.0 L7	SC/SCX/RS/RSX/RI*1 4.1	1
	Implant diameter 4.5				
	57811	■	Ø 5.5 L3	SC/SCX/RS/RSX/RI*1 4.5	1
	57812	■	Ø 5.5 L5	SC/SCX/RS/RSX/RI*1 4.5	1
	58152	■	Ø 5.5 L7	SC/SCX/RS/RSX/RI*1 4.5	1
	Implant diameter 5.5				
	57813	■	Ø 6.5 L3	SC/SCX/RS/RSX/RI*1 5.5	1
	57814	■	Ø 6.5 L5	SC/SCX/RS/RSX/RI*1 5.5	1
	58153	■	Ø 6.5 L7	SC/SCX/RS/RSX/RI*1 5.5	1



*1 New version of the BEGO Semados® RI implants, with Platform Switch Design


*2 For torque specifications, see page 124

*5 Platform Switch Design


Healing posts Platform Switch						
Description	REF	Colour code	Size	Compatibility		Units
PS HPW prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	Implant diameter 3.25–3.75					
	57815		Ø 5.5 L3	SC/SCX/RS/R SX/RI*1	3.25–3.75	1
	58200		Ø 5.5 L5	SC/SCX/RS/R SX/RI*1	3.25–3.75	1
	58201		Ø 5.5 L7	SC/SCX/RS/R SX/RI*1	3.25–3.75	1
	Implant diameter 4.1					
	57816		Ø 6.0 L3	SC/SCX/RS/R SX/RI*1	4.1	1
	58202		Ø 6.0 L5	SC/SCX/RS/R SX/RI*1	4.1	1
	58203		Ø 6.0 L7	SC/SCX/RS/R SX/RI*1	4.1	1
	Implant diameter 4.5					
	57817		Ø 6.5 L3	SC/SCX/RS/R SX/RI*1	4.5	1
	58204		Ø 6.5 L5	SC/SCX/RS/R SX/RI*1	4.5	1
	58205		Ø 6.5 L7	SC/SCX/RS/R SX/RI*1	4.5	1
	Implant diameter 5.5					
	57818		Ø 7.0 L3	SC/SCX/RS/R SX/RI*1	5.5	1
	58206		Ø 7.0 L5	SC/SCX/RS/R SX/RI*1	5.5	1
	58207		Ø 7.0 L7	SC/SCX/RS/R SX/RI*1	5.5	1





Healing posts						
Description	REF	Colour code	Size	Compatibility		Units
Healing post, individual customisable gingival former comprising: • healing post • prosthesis screw Hex 1.25 mm Material: Polyetheretherketone (PEEK) Tool: Hexagon screwdriver 1.25 mm *2	55953		Ø 7.0	S / SC/SCX/RS/R SX/RI	3.25–5.5	1



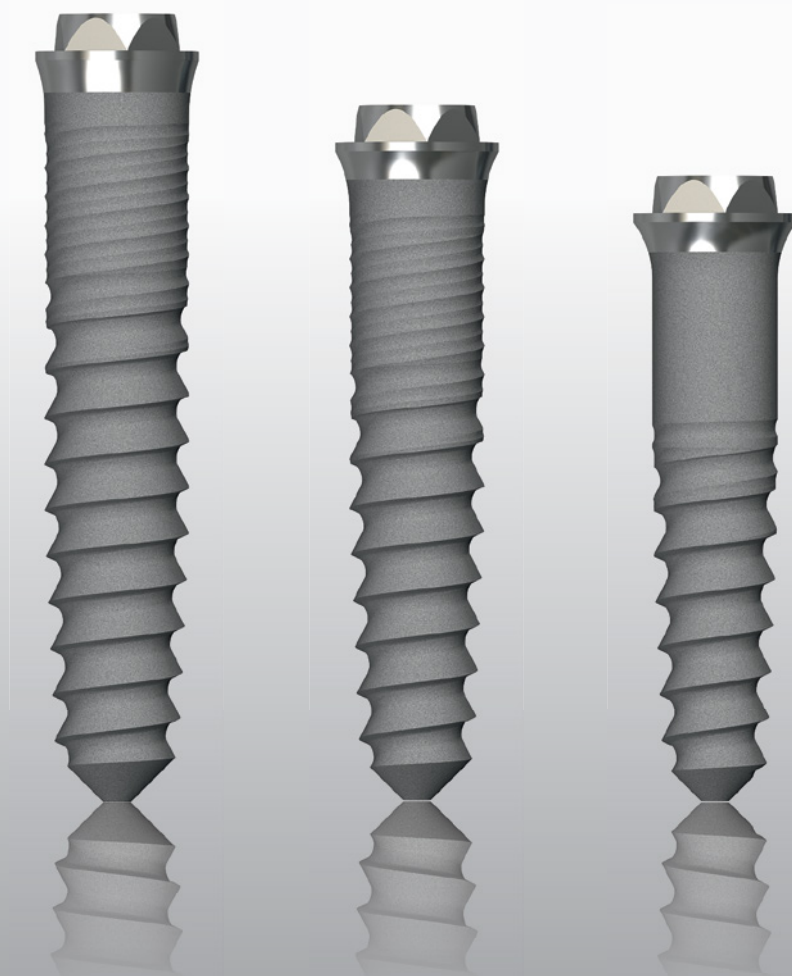

DESCRIPTION

The BEGO Semados® Mini implant is a bone-condensing, non-self-tapping implant made of pure titanium (grade 4).

BEGO Semados® Mini implants 2.7–3.1 can be used together with a bar joint restoration. At least 4 implants should be placed in the edentulous mandible and between 4 and 6 in the maxilla. For bar restorations, it is recommended to use a diameter of 3.1 for the terminal implants.

BEGO Semados® Mini implants 2.7 and 3.1 can be used together with a ball attachment restoration. Two implants should be placed in each jaw.













Only BEGO Semados® Mini implants 3.1 are approved for restorations with Easy-Con Mini abutments. Use 2–4 implants in this case.



For restoring narrow gaps in the anterior teeth following the loss of teeth 12, 22, 32, 31, 41 and 42, the BEGO Semados® Mini 2.9 and 3.1 can be used.





Regardless of the apical diameter, every BEGO Semados® Mini implant has a platform diameter of 3.5 mm.



Consult instructions for use

Implants						
Description	REF	Colour code	Size	Compatibility	Units	
BEGO Semados® implants incl. cover screw and titanium insertion posts TiPure ^{plus} surface Material: Titanium grade 4 (packaged sterile)	56947		2.7 L11.5	Mini	1	
	56948		2.7 L13	Mini	1	
	56949		2.7 L15	Mini	1	
	56950		2.9 L11.5	Mini	1	
	56951		2.9 L13	Mini	1	
	56952		2.9 L15	Mini	1	
	56953		3.1 L11.5	Mini	1	
	56954		3.1 L13	Mini	1	
	56955		3.1 L15	Mini	1	

Cover screws						
Description	REF	Colour code	Size	Compatibility	Units	
Implant cover screw Mini Material: Titanium grade 4 (packaged sterile) Tool: Hexagon screwdriver 1.25 mm *2	56956		L2	Mini 2.7–3.1	1	

Healing posts						
Description	REF	Colour code	Size	Compatibility	Units	
Healing posts Mini prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	56957		Ø3.5 L3	Mini 2.7–3.1	1	
	56958		Ø3.5 L4	Mini 2.7–3.1	1	
	57252		Ø3.5 L7	Mini 2.7–3.1	1	

*2 For torque specifications, see page 124



DESCRIPTION

The BEGO Semados® provisional implant (PI) is a self-tapping, temporary implant made of grade 5 titanium that is not suitable for osseointegration or long-term fixation > 12 months due to its untreated surface.

BEGO Semados® provisional implants can be used in both partially and fully edentulous patients. They are used exclusively for temporary treatment (< 12 months) for one of the following applications:

- Stabilising bridges or dentures during the healing phase of the definitive implants
- Relieving loads on augmented areas and soft tissue
- Interim restoration
- Fixing templates during guided surgery

Implants					
Description	REF	Colour code	Size	Compatibility	Units
BEGO Semados® Provisional Implant (PI) Material: Titanium alloy (packaged sterile)	57660		Ø2.8 L14		1
	57673		Ø2.8 L14		10



Surgical tray					
Description	REF	Colour code	Size	Compatibility	Units
BEGO Semados® PI Tray incl. container, fully equipped	57670				1



Impression taking					
Description	REF	Colour code	Size	Compatibility	Units
PI multifunctional cap Material: Titanium alloy	57661				1
	57674				5



Female parts					
Description	REF	Colour code	Size	Compatibility	Units
PI multifunctional cap Material: Titanium alloy	57661				1
	57674				5
PI protection cap Material: Polyetheretherketone (PEEK) (packaged sterile)	57662				5



Implant analog					
Description	REF	Colour code	Size	Compatibility	Units
PI implant analog	57671				1



Instruments					
Description	REF	Colour code	Size	Compatibility	Units
PI depth drill	57664		Ø 1.5 L20		1
PI paralleling post	57663				1
PI insertion tool with W&H contra-angle connection	57665				1
BEGO Semados® ratchet adapter with ratchet connection for univer- sal use of the ratchet (ratchet grips the adapter head / adapter shaft holds the dental shaft as described in EN ISO 1797-1)	55599				1
PI removal tool	57666				1
PI ratchet	57668				1
PI bending instrument	57667				1
PI stabiliser	57669				1





OVERVIEW

BEGO Guide System S-Line (S/SC/SCX implants)

38

BEGO Guide System RS/RSX-Line

41

BEGO Guide System S-Line (S/SC/SCX implants)

Tray for guided surgery

Description	REF	Colour code	Size	Compatibility	Units
BEGO Guide S-Line tray incl. container, fully equipped	57399			S-Line	1



Master sleeves for guided surgery

Description	REF	Colour code	Size	Compatibility	Units
BEGO Guide master sleeves	57395		Ø 4.2 (A)	S/RS/RSX-Line	10
	57397		Ø 4.7 (B)	S/RS/RSX-Line	10



Reduction sleeves for guided surgery

Description	REF	Colour code	Size	Compatibility	Units
BEGO Guide spoons	57411		Ø 1.6 (A1)	S-Line	1
	57412		Ø 2.5 (A2)	S-Line	1
	57413		Ø 2.8 (A3)	S / SC / SCX 3.25	1
	57414		Ø 3.25 (A4)	S / SC / SCX 3.75	1
	57415		Ø 1.6 (B1)	S-Line	1
	57416		Ø 2.5 (B2)	S-Line	1
	57417		Ø 2.8 (B3)	S / SC / SCX 3.25	1
	57418		Ø 3.25 (B4)	S / SC / SCX 3.75	1
	57419		Ø 3.65 (B5)	S / SC / SCX 4.1	1
	57420		Ø 4.0 (B6)	S / SC / SCX 4.5	1











Tissue punches for guided surgery

Description	REF	Colour code	Size	Compatibility	Units
BEGO Guide tissue punches	57421	□ ■ ■	Ø 4.2 (A)	S / SC / SCX / RS / RSX 3.0–3.75	1
	57422	■ ■	Ø 4.7 (B)	S / SC / SCX / RS / RSX 4.1–4.5	1







Note: BEGO Guide System S-Line – template-guided preparation of BEGO Semados® S/SC/SCX implants 3.25–4.5 is possible.

BEGO Guide System S-Line (S/SC/SCX implants)

Preparation instruments for guided surgery							
Description	REF	Colour code	Size	Compatibility		Units	
BEGO Guide centre drill	57459		Ø 4.2 (A)	S / SC/SCX/RS/RSX	3.0-3.75	1	
	57463		Ø 4.7 (B)	S / SC/SCX/RS/RSX	4.1-4.5	1	
BEGO Guide pilot drill	57423		Ø 1.6 L18 (X1)	S-Line		1	
	57424		Ø 1.6 L23.5 (Y1)	S-Line		1	
	57425		Ø 1.6 L29 (Z1)	S-Line		1	
BEGO Guide depth drill	57426		Ø 2.5 L18 (X2)	S-Line		1	
	57427		Ø 2.5 L23.5 (Y2)	S-Line		1	
	57428		Ø 2.5 L29 (Z2)	S-Line		1	
BEGO Guide depth drill	57429	■	Ø 2.8 L18 (X3)	S / SC / SCX	3.25	1	
	57430	■	Ø 2.8 L23.5 (Y3)	S / SC / SCX	3.25	1	
	57431	■	Ø 2.8 L29 (Z3)	S / SC / SCX	3.25	1	
BEGO Guide depth drill	57432	■	Ø 3.25 L18 (X4)	S / SC / SCX	3.75	1	
	57433	■	Ø 3.25 L23.5 (Y4)	S / SC / SCX	3.75	1	
	57434	■	Ø 3.25 L29 (Z4)	S / SC / SCX	3.75	1	
BEGO Guide depth drill	57435	■	Ø 3.65 L18 (X5)	S / SC / SCX	4.1	1	
	57436	■	Ø 3.65 L23.5 (Y5)	S / SC / SCX	4.1	1	
	57437	■	Ø 3.65 L29 (Z5)	S / SC / SCX	4.1	1	
BEGO Guide depth drill	57438	■	Ø 4.0 L18 (X6)	S / SC / SCX	4.5	1	
	57439	■	Ø 4.0 L23.5 (Y6)	S / SC / SCX	4.5	1	
	57441	■	Ø 4.0 L29 (Z6)	S / SC / SCX	4.5	1	
BEGO Guide countersink	57442	■	(3)	S / SC / SCX	3.25	1	
	57443	■	(4)	S / SC / SCX	3.75	1	
	57444	■	(5)	S / SC / SCX	4.1	1	
	57445	■	(6)	S / SC / SCX	4.5	1	

BEGO Guide System S-Line (S/SC/SCX implants)

Preparation instruments for guided surgery					
Description	REF	Colour code	Size	Compatibility	Units
BEGO Guide screw tapper	57446		(3)	S / SC / SCX 3.25	1
	57447		(4)	S / SC / SCX 3.75	1
	57448		(5)	S / SC / SCX 4.1	1
	57449		(6)	S / SC / SCX 4.5	1



Connector for guided surgery					
Description	REF	Colour code	Size	Compatibility	Units
BEGO Guide connector	57450		Ø 4.2 (AX)	S-Line	1
	57451		Ø 4.2 (AY)	S-Line	1
	57452		Ø 4.2 (AZ)	S-Line	1
	57453		Ø 4.7 (BX)	S-Line	1
	57454		Ø 4.7 (BY)	S-Line	1
	57455		Ø 4.7 (BZ)	S-Line	1
BEGO Guide depth stock ring connector	57456		Ø 4.2 (A)	S/RS/RSX-Line	1
	57457		Ø 4.7 (B)	S/RS/RSX-Line	1
BEGO Guide ratchet adapter for connector	57458			S-Line	1



Note: BEGO Guide System S-Line – template-guided preparation of BEGO Semados® S/SC/SCX implants 3.25–4.5 is possible.

Note: BEGO Guide System RS / RSX-Line – template-guided preparation of BEGO Semados® RS/RSX implants 3.0–4.5 is possible.

BEGO Guide System RS/RSX-Line

Tray for guided surgery

Description	REF	Colour code	Size	Compatibility	Units
BEGO Guide tray incl. container, fully equipped	58071			RS/RSX-Line	1



Master sleeves for guided surgery

Description	REF	Colour code	Size	Compatibility	Units
BEGO Guide master sleeves	57395		Ø 4.2 (A)	S/RS/RSX-Line	10
	57397		Ø 4.7 (B)	S/RS/RSX-Line	10





Reduction sleeves for guided surgery

Description	REF	Colour code	Size	Compatibility	Units
BEGO Guide spoon	57686		Ø 2.0 (A1)	RS/RSX-Line	1
	57687		Ø 2.5 (A2)	RS/RSX-Line	1
	57688		Ø 2.8 (A3)	RS/RSX 3.0	1
	57689		Ø 3.4 (A4)	RS/RSX 3.75	1
	57690		Ø 2.0 (B1)	RS/RSX-Line	1
	57691		Ø 2.5 (B2)	RS/RSX-Line	1
	57692		Ø 2.8 (B3)	RS/RSX 3.0	1
	57693		Ø 3.4 (B4)	RS/RSX 3.75	1
	57694		Ø 3.8 (B5)	RS/RSX 4.1	1
	57695		Ø 4.1 (B6)	RS/RSX 4.5	1



Tissue punches for guided surgery

Description	REF	Colour code	Size	Compatibility	Units
BEGO Guide tissue punches	57421		Ø 4.2 (A)	S / SC/SCX/RS/RSX 3.0–3.75	1
	57422		Ø 4.7 (B)	S / SC/SCX/RS/RSX 4.1–4.5	1



BEGO Guide System RS/RSX-Line

Preparation instruments for guided surgery						
Description	REF	Colour code	Size	Compatibility		Units
BEGO Guide centre drill	57459		Ø 4.2 (A)	S / SC/SCX/RS/RSX	3.0–3.75	1
	57463		Ø 4.7 (B)	S / SC/SCX/RS/RSX	4.1–4.5	1
BEGO Guide PD pilot drill for guided surgery	57696		Ø 2.0 L18 (X1)	RS/RSX-Line		1
	57697		Ø 2.0 L23.5 (Y1)	RS/RSX-Line		1
	57698		Ø 2.0 L29 (Z1)	RS/RSX-Line		1
BEGO Guide DD depth drill for guided surgery	57713		Ø 2.5 L18 (X2)	RS/RSX-Line		1
	57714		Ø 2.5 L23.5 (Y2)	RS/RSX-Line		1
	57715		Ø 2.5 L29 (Z2)	RS/RSX-Line		1
BEGO Guide DD depth drill for guided surgery	57716	□	Ø 2.8 L18 (X3)	RS/RSX	3.0	1
	57717	□	Ø 2.8 L23.5 (Y3)	RS/RSX	3.0	1
	57723	□	Ø 2.8 L29 (Z3)	RS/RSX	3.0	1
BEGO Guide DD depth drill for guided surgery	57724	■	Ø 3.4 L18 (X4)	RS/RSX	3.75	1
	57725	■	Ø 3.4 L23.5 (Y4)	RS/RSX	3.75	1
	57726	■	Ø 3.4 L29 (Z4)	RS/RSX	3.75	1
BEGO Guide DD depth drill for guided surgery	57727	■	Ø 3.8 L18 (X5)	RS/RSX	4.1	1
	57733	■	Ø 3.8 L23.5 (Y5)	RS/RSX	4.1	1
	57734	■	Ø 3.8 L29 (Z5)	RS/RSX	4.1	1
BEGO Guide DD depth drill for guided surgery	57735	■	Ø 4.1 L18 (X6)	RS/RSX	4.5	1
	57736	■	Ø 4.1 L23.5 (Y6)	RS/RSX	4.5	1
	57737	■	Ø 4.1 L29 (Z6)	RS/RSX	4.5	1
BEGO Guide CS countersink for guided surgery	58051	□	(3)	RS/RSX	3.0	1
	58052	■	(4)	RS/RSX	3.75	1
	58053	■	(5)	RS/RSX	4.1	1
	58054	■	(6)	RS/RSX	4.5	1

Note: BEGO Guide System RS / RSX-Line – template-guided preparation of BEGO Semados® RS/RSX implants 3.0–4.5 is possible.

BEGO Guide System RS/RSX-Line

Preparation instruments for guided surgery

Description	REF	Colour code	Size	Compatibility	Units
BEGO Guide ST screw tapper for guided surgery	58055	□	(3)	RS/RSX 3.0	1
	58056	■	(4)	RS/RSX 3.75	1
	58057	■	(5)	RS/RSX 4.1	1
	58058	■	(6)	RS/RSX 4.5	1





Connector for guided surgery

Description	REF	Colour code	Size	Compatibility	Units
BEGO Guide connector with contra-angle connection	58059		Ø 4.2 (AX)	RS/RSX-Line	1
	58060		Ø 4.2 (AY)	RS/RSX-Line	1
	58061		Ø 4.2 (AZ)	RS/RSX-Line	1
	58062		Ø 4.7 (BX)	RS/RSX-Line	1
	58063		Ø 4.7 (BY)	RS/RSX-Line	1
	58064		Ø 4.7 (BZ)	RS/RSX-Line	1
BEGO Guide connector with ratchet connection	58065		Ø 4.2 (AX)	RS/RSX-Line	1
	58066		Ø 4.2 (AY)	RS/RSX-Line	1
	58067		Ø 4.2 (AZ)	RS/RSX-Line	1
	58068		Ø 4.7 (BX)	RS/RSX-Line	1
	58069		Ø 4.7 (BY)	RS/RSX-Line	1
	58070		Ø 4.7 (BZ)	RS/RSX-Line	1
BEGO Guide depth stock ring connector	57456		Ø 4.2 (A)	S/RS/RSX-Line	1
	57457		Ø 4.7 (B)	S/RS/RSX-Line	1



BEGO Guide System - guided pilot drill holes

Preparation instruments for guided surgery					
Description	REF	Colour code	Size	Compatibility	Units
BEGO Guide pilot drill for guided surgical pilot drill holes	57400		Ø 2.0 L22		1
	57401		Ø 2.0 L30		1
					





Drill sleeves for guided surgery					
Description	REF	Colour code	Size	Compatibility	Units
BEGO Guide DS for guided surgical pilot drill holes	57130		Ø 2.0		10
					



OVERVIEW

Preparation instruments for S-Line (S/SC/SCX implants)	46
Preparation instruments for RS/RSX-Line	49
Preparation instruments for RI-Line	52
Preparation instruments for Mini-Line	55
Bone shapers/trepans	56
Surgical instruments	57


BEGO Semados® S-Line (S/SC/SCX implants)

Tissue punches						
Description	REF	Colour code	Size	Compatibility		Units
Tissue punches	57056			S / SC/SCX/RS/R SX/RI	3.25–3.75	1
	57057			S / SC/SCX/RS/R SX/RI	4.1	1
	57058			S / SC/SCX/RS/R SX/RI	4.5	1
	57059			S / SC/SCX/RS/R SX/RI	5.5	1



Surgical tray						
Description	REF	Colour code	Size	Compatibility		Units
BEGO Semados® S-Line tray^{Plus} incl. container, excl. drill module Ø 5.5 (REF 57347)	57340			S-Line		1


























Drill module						
Description	REF	Colour code	Size	Compatibility		Units
Drill module comprising: • depth drill, short • countersink • screw tapper with ratchet connection	57347			S / SC / SCX	5.5	1










Preparation Instruments						
Description	REF	Colour code	Size	Compatibility		Units
Pilot marker	57308		Ø 1.6 L15	S-Line		1
	57309		Ø 1.6 L23	S-Line		1
Pilot drill Alternative item to pilot marker	55752		Ø 1.6 L16	S-Line		1
	55811		Ø 1.6 L24	S-Line		1
Depth drill 2.5	57100		Ø 2.5 L15	S-Line		1
	57101		Ø 2.5 L20	S-Line		1



BEGO Semados® S-Line (S/SC/SCX implants)

Preparation Instruments						
Description	REF	Colour code	Size	Compatibility	Units	
Depth drill	57102		Ø 2.8 L15	S / SC / SCX 3.25	1	
	57104		Ø 3.25 L15	S / SC / SCX 3.75	1	
	57106		Ø 3.65 L15	S / SC / SCX 4.1	1	
	57108		Ø 4.0 L15	S / SC / SCX 4.5	1	
	57110		Ø 4.7 L15	S / SC / SCX 5.5	1	
Depth drill	57103		Ø 2.8 L20	S / SC / SCX 3.25	1	
	57105		Ø 3.25 L20	S / SC / SCX 3.75	1	
	57107		Ø 3.65 L20	S / SC / SCX 4.1	1	
	57109		Ø 4.0 L20	S / SC / SCX 4.5	1	
Countersink	57350			S / SC / SCX 3.25	1	
	57351			S / SC / SCX 3.75	1	
	57352			S / SC / SCX 4.1	1	
	57353			S / SC / SCX 4.5	1	
	57354			S / SC / SCX 5.5	1	
Screw tapper	57332			S / SC / SCX 3.25	1	
	57333			S / SC / SCX 3.75	1	
	57334			S / SC / SCX 4.1	1	
	57335			S / SC / SCX 4.5	1	
	57336			S / SC / SCX 5.5	1	

BEGO Semados® S-Line (S/SC/SCX implants)

Drill stop sets						
Description	REF	Colour code	Size	Compatibility	Number	
Drill stops	55804			Depth drill 2.5 and S/SC/SCX 3.25–3.75	1 set	
	55715			S / SC / SCX 4.1	1 set	
	55810			S / SC / SCX 4.5	1 set	
	55910			S / SC / SCX 5.5	1 set	
Drill stop tray ^{Plus} incl. storage box, lid and all drill stops	57345			S-Line	1 unit	

New
design
available from
Q3/17







**New
design**
available from
Q3/17



BEGO Semados® RS/RSX-Line

Tissue punches

Description	REF	Colour code	Size	Compatibility	Units
Tissue punches	57056			S / SC/SCX/RS/RSX/RI 3.25–3.75	1
	57057			S / SC/SCX/RS/RSX/RI 4.1	1
	57058			S / SC/SCX/RS/RSX/RI 4.5	1
	57059			S / SC/SCX/RS/RSX/RI 5.5	1




Surgical tray

Description	REF	Colour code	Size	Compatibility	Units
BEGO Semados® RS/RSX-Line tray^{Plus} incl. container, excl. drill module Ø 5.5 (REF 57948)	57949			RS/RSX-Line	1



Drill module

Description	REF	Colour code	Size	Compatibility	Units
Drill module comprising: • depth drill, short • DD D1 (depth drill) • countersink • screw tapper	57948			RS/RSX 5.5	1








Preparation Instruments

Description	REF	Colour code	Size	Compatibility	Units
Pilot marker	57481		Ø 1.6 L15	RS/RSX-Line	1
	57482		Ø 1.6 L23	RS/RSX-Line	1
Depth drill 2.5	57926		Ø 2.5 L15	RS/RSX-Line	1
	57927		Ø 2.5 L20	RS/RSX-Line	1



BEGO Semados® RS/RSX-Line

Preparation Instruments						
Description	REF	Colour code	Size	Compatibility		Units
Depth drill	57928	□	Ø 2.8 L15	RS/RSX 3.0		1
	57930	■	Ø 3.4 L15	RS/RSX 3.75		1
	57932	■	Ø 3.8 L15	RS/RSX 4.1		1
	57934	■	Ø 4.1 L15	RS/RSX 4.5		1
	57936	■	Ø 5.0 L15	RS/RSX 5.5		1
						
DD D1 (depth drill) Alternative item to the depth drill RS/RSX-Line short, for optional use only for exceptionally compact bone, particularly in the mandible.	57484	□	Ø 2.9 L15	RS/RSX 3.0		1
	57485	■	Ø 3.6 L15	RS/RSX 3.75		1
	57486	■	Ø 4.0 L15	RS/RSX 4.1		1
	57487	■	Ø 4.3 L15	RS/RSX 4.5		1
	57488	■	Ø 5.3 L15	RS/RSX 5.5		1
						
Depth drill	57929	□	Ø 2.8 L20	RS/RSX 3.0		1
	57931	■	Ø 3.4 L20	RS/RSX 3.75		1
	57933	■	Ø 3.8 L20	RS/RSX 4.1		1
	57935	■	Ø 4.1 L20	RS/RSX 4.5		1
						
Countersink	57937	□		RS/RSX 3.0		1
	57938	■		RS/RSX 3.75		1
	57939	■		RS/RSX 4.1		1
	57940	■		RS/RSX 4.5		1
	57941	■		RS/RSX 5.5		1
						
Screw tapper	57943	□		RS/RSX 3.0		1
	57944	■		RS/RSX 3.75		1
	57945	■		RS/RSX 4.1		1
	57946	■		RS/RSX 4.5		1
	57947	■		RS/RSX 5.5		1
						

BEGO Semados® RS/RSX-Line





Drill stop sets					
Description	REF	Colour code	Size	Compatibility	Number
Drill stops	57476		Depth drill 2.5	RS/RSX-Line	1 set
	57477	□		RS/RSX 3.0	1 set
	57478	■		RS/RSX 3.75	1 set
	57479	■ ■		RS/RSX 4.1–4.5	1 set
	57480	■		RS/RSX 5.5	1 set
Drill stop tray ^{Plus} incl. storage box, lid and all drill stops	57483	□ ■ ■ ■ ■		RS/RSX-Line	1 unit



**New
design**
available from
Q3/17

BEGO Semados® RI-Line

Tissue punches

Description	REF	Colour code	Size	Compatibility	Units
Tissue punches	57056			S / SC/SCX/RS/R SX/RI 3.25–3.75	1
	57057			S / SC/SCX/RS/R SX/RI 4.1	1
	57058			S / SC/SCX/RS/R SX/RI 4.5	1
	57059			S / SC/SCX/RS/R SX/RI 5.5	1




Surgical tray

Description	REF	Colour code	Size	Compatibility	Units
BEGO Semados® RI-Line Tray ^{Plus} incl. container, excl. drill module Ø 5.5 (REF 57613)	57612			RI-Line	1



Drill module

Description	REF	Colour code	Size	Compatibility	Units
Drill module comprising: • depth drill • countersink • thread former • screw tapper	57613			RI 5.5	1




























Preparation Instruments

Description	REF	Colour code	Size	Compatibility	Units
Pilot marker	57581		Ø 2.5 L16	RI-Line	1
	57582		Ø 2.5 L25	RI-Line	1
Depth drill 3.2	57583		Ø 3.2 L15	RI-Line	1
	57584		Ø 3.2 L20	RI-Line	1



BEGO Semados® RI-Line

Preparation Instruments						
Description	REF	Colour code	Size	Compatibility		Units
Depth drill	57585		Ø 3.52 L15	RI	3.75	1
	57587		Ø 3.93 L15	RI	4.1	1
	57589		Ø 4.32 L15	RI	4.5	1
	57591		Ø 5.28 L15	RI	5.5	1
						
Depth drill	57586		Ø 3.52 L20	RI	3.75	1
	57588		Ø 3.93 L20	RI	4.1	1
	57590		Ø 4.32 L20	RI	4.5	1
						
Countersink	57592			RI	3.75	1
	57593			RI	4.1	1
	57594			RI	4.5	1
	57595			RI	5.5	1
						
Thread former	55766			RI	3.25	1
	57615			RI	3.75	1
	57616			RI	4.1	1
	57617			RI	4.5	1
	57618			RI	5.5	1
						
Screw taper	57619			RI	3.75	1
	57620			RI	4.1	1
	57621			RI	4.5	1
	57622			RI	5.5	1
						

BEGO Semados® RI-Line

Drill stop sets					
Description	REF	Colour code	Size	Compatibility	Number
Drill stops	57607		Depth drill 3.2	RI-Line	1 set
	57608	■ ■		RI 3.75–4.1	1 set
	57609	■ ■		RI 4.5–5.5	1 set
Drill stop tray ^{Plus} incl. storage box, lid and all drill stops	57610	■ ■ ■ ■		RI-Line	1 unit



New
design
available from
Q3/17

BEGO Semados® Mini-Line

Surgical tray					
Description	REF	Colour code	Size	Compatibility	Units
Mini-/Osseo ^{Plus} tray incl. container, fully equipped	56970			Mini-Line	1







Preparation Instruments					
Description	REF	Colour code	Size	Compatibility	Units
Initial drill	55714				1
DD (depth drill)	57995	■ ■	Ø 2.55 L16.5	Mini 2.7	1
	57996	■ ■	Ø 2.75 L16.5	Mini 2.9	1
	57997	■ ■	Ø 2.95 L16.5	Mini 3.1	1
Thread former	56979	■ ■		Mini 2.7	1
	56980	■ ■		Mini 2.9	1
	56981	■ ■		Mini 3.1	1



Optional preparation instruments					
Description	REF	Colour code	Size	Compatibility	Units
Gap-cutter disc	56985				1
Gap-cutter drill	56986				1











Bone shaper					
Description	REF	Colour code	Size	Compatibility	Units
Bone profiler	57467			S / RI 3.25–3.75	1
	57468			S / RI 4.1	1
	57469			S / RI 4.5	1
	57470			S / RI 5.5	1



Trepan drill					
Description	REF	Colour code	Size	Compatibility	Units
Trepan drill	55817		Ø 4.2 external / Ø 3.7 internal	L20	1
	55815		Ø 5.0 external / Ø 4.1 internal	L20	1
	56991		Ø 5.0 external / Ø 4.3 internal	L20	1
	55816		Ø 6.0 external / Ø 5.1 internal	L20	1



Surgical Instruments						
Description	REF	Colour code	Size	Compatibility	Units	
Drill extension one-part without internal cooling	57265		Extension by 15.8 mm		1	
Insertion tool for implants with ratchet connection	55831		L6		1	
	55830		L12.5		1	
Insertion tool for implants with contra-angle connection	56990		L21.5		1	
	55832		L24		1	
IDC (implant adjustment instrument) for making final corrections to the position of the inserted implant after removing the insertion post	56749			RS/RSX 3.0	1	
	56748			S/SC/SCX/RS/RSX/RI 3.25–5.5	1	
Guiding wrench open-end spanner and guide pin for tools with ratchet connection	53897				1	
Paralleling post	55863			S-Line	2	
	57956			RS/RSX-Line	2	
	57598			RI-Line	1	
	56972			Mini-Line	1	

Surgical Instruments					
Description	REF	Colour code	Size	Compatibility	Units
Depth gauge	53872			S-Line	1
	55746			RI-Line	1
	57955			RS/RSX-Line	1
Fibreglass pen for removing dried contamination from the instruments	55523				1
Replacement brush for the fibreglass pen (image shows the entire Fibreglass pen)	55524				1
Ratchet / torque wrench With torques 10–50 Ncm	55799				1
BEGO Semados® ratchet adapter with ratchet connection for univer- sal use of the ratchet (ratchet grips the adapter head / adapter shaft holds the dental shaft as described in EN ISO 1797-1)	55599				1



*1 New version of the BEGO Semados RI implants, with Platform Switch Design



OVERVIEW

Prosthetic Instruments	60
CAD/CAM Implant Prosthetics from Bego Medical	61
Prosthetics SC/SCX/RS/R SX/RI* ¹ with Platform Switch Design	67
Prosthetics Mini-Line	91
BEGO Semados S / RI Implants without Platform Switch Design	101


Prosthetic tray					
Description	REF	Colour code	Size	Compatibility	Units
Prosthetic kit with ratchet / torque wrench, hexagon screwdriver 1.25 mm short / long, slot screwdriver long, insertion tool for ball attachment, insertion tool 3Locator®, ratchet adapter, incl. storage box and cover	55826				1

**New
design**
available from
Q3 / 17



Prosthetic Instruments					
Description	REF	Colour code	Size	Compatibility	Units
Hexagon screwdriver 1.25 mm with conical ratchet connection for implant cover screws, healing posts, cover posts, inser- tion posts and prosthesis screws	57266		L5		1
	53949		L10		1
	53948		L17		1
Hexagon screwdriver 1.25 mm, contra-angle conical for implant cover screws, healing posts, impression posts, insertion posts and prosthesis screws	55563		L25		1
	55564		L31		1
Slot screwdriver with ratchet connection For technician screws, healing posts and insertion posts	53953		L10		1
	53952		L14		1
Ratchet / torque wrench with torques 10–50 Ncm	55799				1
BEGO Semados® ratchet adapter with ratchet connection for univer- sal use of the ratchet (ratchet grips the adapter head / adapter shaft holds the dental shaft as described in EN ISO 1797-1)	55599				1



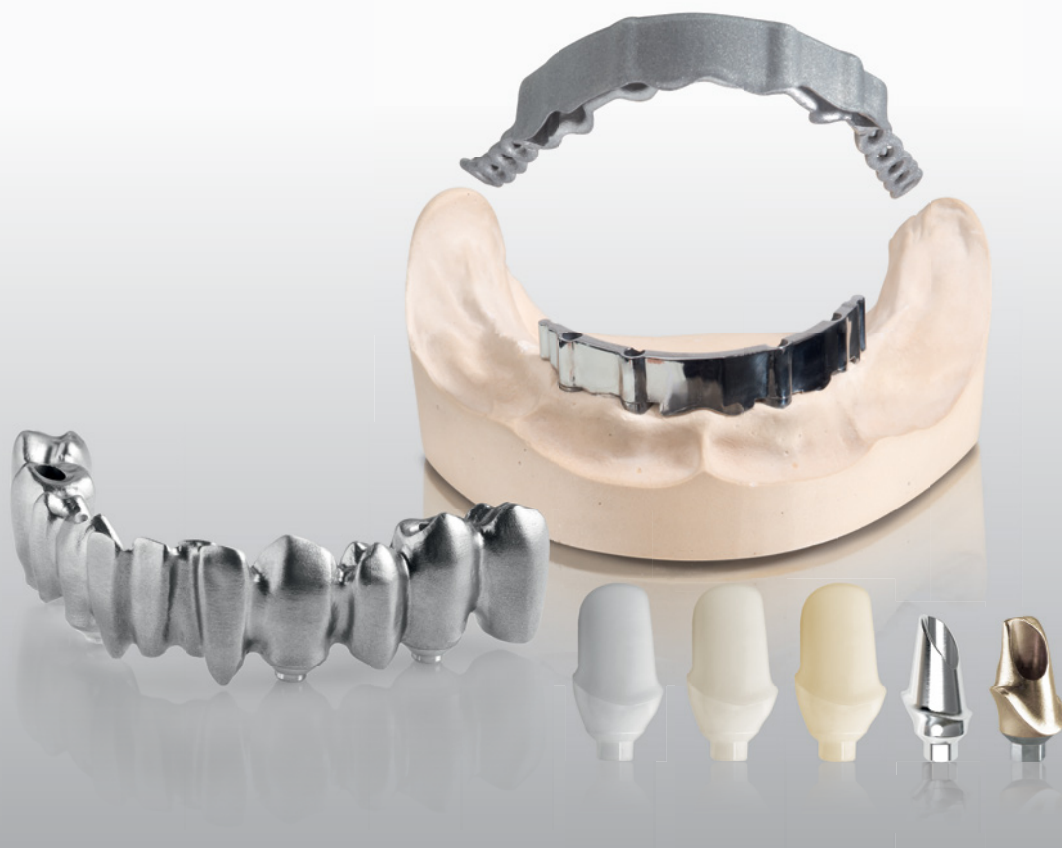

OVERVIEW

Interface summary	62
BEGO CADAbut F –one-part individual healing posts	62
BEGO CADAbut D –two-part individual healing posts	62
BEGO CADAbut F –one-part individual abutments	63
BEGO CADAbut D –two-part individual abutments	63
BEGO CADBase (bar bases)	64
BEGO CADBar	64
Additional holding elements	65
Bar secondary structure	65
Bridge bases	66
Zirconia Maryland bridges	66

Interface summary



CADAbut F



CADAbut D


CADBase
Implant
Level

CADBase
Abutment
Level

Diameter	Platform	BEGO titanium grade 5	Wirobond® MI+	BeCe® CAD Zirkon XH	IPS e.max CAD	BEGO Zirkon LT	BEGO PMMA Multicolor	CAD/Cast® alloys	Wirobond® C+	BEGO Zirkon LT Maryland bridge	BEGO titanium grade 5	Wirobond® MI+	BEGO titanium grade 5	Wirobond® MI+

BEGO Implant Systems – Semados® S/RI-Line (without Platform Switch)

3.25; 3.75	3.67													
4.1	4.1	√ *A *B	√ *A *B	√ *A *B	√ *A *B	√ *A *B	√ *A *B	√ *A *B	√ *A *B	√ *A *B	√ *A *B	√ *A *B	√ *A *B	√ *A *B
4.5	4.5													
5.5	5.5													

BEGO Implant Systems – Semados® SC / SCX / RS / RSX/RI*1, PS-Line (with Platform Switch)

3.0	3.0													
3.25; 3.75	3.67													
4.1	4.1	√ *A *B		√ *A *B	√ *A *B	√ *A *B	√ *A *B	√ *A *B		√ *A *B	√ *A *B	√ *A *B	√ *A *B	√ *A *B
4.5	4.5													
5.5	5.5													


BEGO Implant Systems – Semados® Mini-Line

2.7; 2.9; 3.1	3.5										√ *A *B	√ *A *B		
---------------	-----	--	--	--	--	--	--	--	--	--	---------	---------	--	--


BEGO Implant Systems – Semados® MultiPlus

3.25; 3.75; 4.1; 4.5	Abutment level												√ *A *B	√ *A *B
----------------------	----------------	--	--	--	--	--	--	--	--	--	--	--	---------	---------

BEGO CADAbut F – one-part individual healing posts incl prosthesis screw

Description	Units	
BEGO titanium grade 5 only for temporary use	1	

BEGO CADAbut D – two-part individual healing posts (plus titanium adhesive abutment)




Description	Units	
BEGO PMMA Multicolor available in 3 colours (M01, M02, M03), only for temporary use	1	

Note: IPS e.max CAD only available for BEGO Semados® SC/SCX/RS/RSX/RI*1 implants Ø 3.0–5.5 mm.






*A 3Shape *B exocad

*1 New version of the BEGO Semados® RI implants, with Platform Switch Design



BEGO CADAbut F – one-part individual abutments incl prosthesis screw

Description	Units	
BeCe® CAD Zirkon XH available in 3 colours (LL0, LL2, LL3), for anterior restorations only	1	
Wirobond® MI+	1	
BEGO titanium grade 5	1	


BEGO CADAbut D – two-part individual abutments (plus titanium adhesive abutment)

Description	Units	
BEGO Zirkon LT available in 5 colours (LT01–LT05)	1	
IPS e.max CAD Supplied in blue pre-crystallised form. LT can be supplied in 6 colours (A–D). MO supplied in 5 opaque colours.	1	
CAD/Cast® alloys Selected BEGO precious metal alloys at the particular valid daily price, see current price list (tel. +49 421 20 28-251)	1	
Wirobond® C+	1	
BEGO PMMA Multicolor available in 3 colours (M01, M02, M03), only for temporary use	1	








BEGO CADBase (bar bases incl. prosthesis screws)

Description	Number of implant units	
BEGO titanium grade 5	2-4	
	5-7	
	≥ 8	
Wirobond® MI+	2-4	
	5-7	
	≥ 8	

BEGO CADBar

Description	Units	
BEGO titanium grade 5	1	
Wirobond® C+	1	





Bar joint attachments

Description	Cross-section	
Round bar 1.8 mm		
Horix* ⁶ bar 1.8 mm		
Horix* ⁶ bar joint attachment 2.3 mm		
Horix* ⁶ bar joint attachment 3.0 mm		



Indication: Implant/mucosa-retained removable prosthesis on at least two implants (without extensions)


Note: Unfinished bars cannot be obtained from the Scan and Design Centre.


*⁶ This symbol is a commercial name / registered trademark of a business that does not belong to the BEGO Group.


Bar attachment		
Description	Cross-section	
Dolder* ⁶ bar attachment 3.0 mm		
Individual bar shapes / bar attachment		

Indication: Implant-retained removable prosthesis on at least four implants (with extensions)

Additional holding elements		
Description	Units	
Rod attachment Ancora/Preci-Vertex* ⁶ 1.8 mm	1	
Thread drills for retention elements, available for: <ul style="list-style-type: none"> • Zest Anchors*⁶ • CEKA*⁶ attachment M2 • CEKA*⁶ attachment M3 • CEKA*⁶ ball anchor M2 	1	

Retention elements		
Description		
Dolder*⁶ bar female parts also available from ALPHADENT NV, Belgium, www.ceka-preciline.com		

Retention elements		
Description		
Ancora female parts (Preci-Vertex* ⁶ rider/ Preci-Horix* ⁶ rider) also available from ALPHADENT NV, Belgium, www.ceka-preciline.com		

Bar secondary structure		
Description	Units	
Wirobond® C+ regardless of the size, number and shape of the retentions	1	

Bridge based on at least 2 implants		
Description	Number of implant units	Units
BEGO titanium grade 5	2–4	1
	5–7	1
	≥ 8	1
Wirobond® MI+	2–4	1
	5–7	1
	≥ 8	1
Pontic		1



Zirconia adhesive bridge (plus titanium adhesive abutment no Hex) on at least 2 implants		
Description		Units
Adhesive bridge abutment BEGO Zirkon LT available in 5 colours (LT01–LT05)		1
Pontic BEGO Zirkon LT available in 5 colours (LT01–LT05)		1



For questions about individually fabricated CAD / CAM implant prosthetics from BEGO Medical GmbH (procedures or conditions), please contact:

BEGO Medical GmbH
Wilhelm-Herbst-Str. 1 · 28359 Bremen,
Germany

Tel. +49 421 2028-0 · Fax +49 421 2028-174
email info@bego-medical.de · www.bego.com

Note: Bridge constructions not available for BEGO Semados® RS / RSX implants Ø 3.0 and Mini-Line.

*1 New version of the BEGO Semados® RI implants, with Platform Switch Design

*5 Platform Switch Design



OVERVIEW

CAD/CAM restoration	68
One Care Package restoration	71
Impression taking and model fabrication	72
Crown restoration Ø 3.0	73
Crown and bridge restoration	74
Multi ⁱ Plus restoration	80
Hybrid restoration	85
Screws	89

Note: The entire Platform Switch prosthetics range is **not** compatible with the previous S / RI implants (without Platform Switch Design)! Please only use the abutments / components shown from page 99 onwards on these implants.

CAD/CAM restoration Ø 3.0

CAD positioner Platform Switch					
Description	REF	Colour code	Size	Compatibility	Units
PS CADP comprising: <ul style="list-style-type: none"> • PS CAD positioner • prosthesis screw for CAD positioner Platform Switch Ø 3.0 Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25 mm * ²	58250	□		RS/R SX 3.0	1



Adhesive abutment Platform Switch					
Description	REF	Colour code	Size	Compatibility	Units
PS TiB comprising: <ul style="list-style-type: none"> • PS adhesive abutment • prosthesis screw RS/R SX 3.0 • technician screw RS/R SX 3.0 Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver * ²	57781	□		RS/R SX 3.0	1



Scansupport					
Description	REF	Colour code	Size	Compatibility	Units
CAD SP comprising: <ul style="list-style-type: none"> • scansupport • prosthesis screw RS/R SX 3.0 Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm * ²	58190	□		RS/R SX 3.0	1



Note: When using the *⁶Cerec® system a *⁶Cerec/ *⁶InLab Scanbody for *⁶Bluecam (36 units) REF 6431303 or Scanbody for *⁶Omnica™ (36 units) REF 6431329 (Sirona Dental Systems GmbH, Bensheim, Germany) is required.

*¹ New version of the BEGO Semados® RI implants, with Platform Switch Design





*² For torque specifications, see page 124


*⁵ Platform Switch Design

*⁶ This symbol is a commercial name / registered trademark of a business that does not belong to the BEGO Group.

CAD/CAM restoration Ø 3.25–5.5





CAD positioner Platform Switch


Description	REF	Colour code	Size	Compatibility	Units	
PS CADD	58251			SC/SCX/RS/RSX/RI* ¹	3.25–3.75	1
comprising:						
• PS CAD positioner	58252			SC/SCX/RS/RSX/RI* ¹	4.1	1
• prosthesis screw Hex 1.25 mm	58253			SC/SCX/RS/RSX/RI* ¹	4.5	1
Material: Titanium grade 4						
Tool: Hexagon screwdriver 1.25 mm	58254			SC/SCX/RS/RSX/RI* ¹	5.5	1
*2						









Adhesive abutments Platform Switch


Description	REF	Colour code	Size	Compatibility	Units	
PS TiB	57823			SC/SCX/RS/RSX/RI* ¹	3.25–3.75	1
comprising:						
• PS adhesive abutment Hex	57824			SC/SCX/RS/RSX/RI* ¹	4.1	1
• prosthesis screw Sub-Tec ^{Plus}	57825			SC/SCX/RS/RSX/RI* ¹	4.5	1
• technician screw Sub-Tec ^{Plus}						
Material: Titanium alloy	57826			SC/SCX/RS/RSX/RI* ¹	5.5	1
Tool: Hexagon screwdriver 1.25 mm / slot screwdriver						
*2						









Scansupport

Description	REF	Colour code	Size	Compatibility	Units	
CAD SP	58191			S / SC/SCX/RS/RSX/RI	3.25–3.75	1
comprising:						
• scansupport	58192			S / SC/SCX/RS/RSX/RI	4.1	1
• prosthesis screw Sub-Tec ^{Plus}	58193			S / SC/SCX/RS/RSX/RI	4.5	1
Material: Titanium alloy						
Tool: Hexagon screwdriver 1.25 mm	58194			S / SC/SCX/RS/RSX/RI	5.5	1
*2						







CAD/CAM restoration Ø 3.25–5.5

Adhesive abutments Platform Switch						
Description	REF	Colour code	Size	Compatibility		Units
PS TiB NH	57827			SC/SCX/RS/RSX/RI* ¹	3.25–3.75	1
comprising:						
• PS adhesive abutment no Hex	57828			SC/SCX/RS/RSX/RI* ¹	4.1	1
• prosthesis screw Sub-Tec ^{Plus}	57829			SC/SCX/RS/RSX/RI* ¹	4.5	1
• technician screw Sub-Tec ^{Plus}						
Material: Titanium alloy	57830			SC/SCX/RS/RSX/RI* ¹	5.5	1
Tool: Hexagon screwdriver						
1.25 mm / slot screwdriver						
*2						



CAD/CAM milling blank Platform Switch						
Description	REF	Colour code	Size	Compatibility		Units
PS PMB	58326		Ø 11.5	SC/SCX/RS/RSX/RI* ¹	3.25–5.5	1
comprising:						
• milling blank Platform Switch	58226		Ø 16	SC/SCX/RS/RSX/RI* ¹	3.25–5.5	1
• prosthesis screw Sub-Tec ^{Plus}						
• technician screw Sub-Tec ^{Plus}						
Material: Titanium alloy						
Tool: Hexagon screwdriver						
1.25 mm / slot screwdriver						
*2						



Note: A *⁶PreFace® abutment holder is required for the corresponding milling machine. This must be ordered directly from the machine manufacturer. You must follow the manufacturer's instructions.











*¹ New version of the BEGO Semados® RI implants, with Platform Switch Design

*² For torque specifications, see page 124

*⁵ Platform Switch Design


*⁶ This symbol is a commercial name / registered trademark of a business that does not belong to the BEGO Group.

One Care Package restoration

Restoration sets Platform Switch						
Description	REF	Colour code	Size	Compatibility	Units	
PS OCP	58297		GH 1	SC/SCX/RS/RX/RI* ¹	3.25–3.75	1
comprising:						
• OCP abutment	58300		GH 3	SC/SCX/RS/RX/RI* ¹	3.25–3.75	1
• multifunctional cap	58298		GH 1	SC/SCX/RS/RX/RI* ¹	4.1	1
• impression coping	58301		GH 3	SC/SCX/RS/RX/RI* ¹	4.1	1
• laboratory cap for crowns	58299		GH 1	SC/SCX/RS/RX/RI* ¹	4.5	1
• laboratory cap for bridges						
• prosthesis screw Sub-Tec ^{Plus}	58302		GH 3	SC/SCX/RS/RX/RI* ¹	4.5	1
Material: Titanium alloy / polyetheretherketone (PEEK) / polycarbonate (PC) (packaged sterile) Tool: Hexagon screwdriver 1.25 mm *2						
						
Laboratory caps, crown						
Description	REF	Colour code	Size	Compatibility	Units	
LCC	58303				5	
Material: Polycarbonate (PC)						
Laboratory caps, bridge						
Description	REF	Colour code	Size	Compatibility	Units	
LCB	58304				5	
Material: Polycarbonate (PC)						
Implant analog						
Description	REF	Colour code	Size	Compatibility	Units	
OCP A	58305				1	
Material: Titanium alloy						

Impression taking and model fabrication Ø3.0–5.5

Impression sets Platform Switch						
Description	REF	Colour code	Size	Compatibility	Units	
PS CTI impression taking on implant with closed tray comprising: • impression post cap • PS impression post • titanium screw Tool: Hexagon screwdriver 1.25 mm / slot screwdriver* ²	57773	□		RS/RXS 3.0	1	
	58316	■		SC/SCX 3.25	1	
	57799	■		SC/SCX/RS/RXS/RI* ¹ 3.75	1	
	57800	■		SC/SCX/RS/RXS/RI* ¹ 4.1	1	
	57801	■		SC/SCX/RS/RXS/RI* ¹ 4.5	1	
	57802	■		SC/SCX/RS/RXS/RI* ¹ 5.5	1	
PS OTI impression taking on implant with open tray comprising: • PS impression post • titanium screw short/long Tool: Hexagon screwdriver 1.25 mm / slot screwdriver* ²	57774	□		RS/RXS 3.0	1	
	58317	■		SC/SCX 3.25	1	
	57803	■		SC/SCX/RS/RXS/RI* ¹ 3.75	1	
	57804	■		SC/SCX/RS/RXS/RI* ¹ 4.1	1	
	57805	■		SC/SCX/RS/RXS/RI* ¹ 4.5	1	
	57806	■		SC/SCX/RS/RXS/RI* ¹ 5.5	1	

Implant analogs Platform Switch						
Description	REF	Colour code	Size	Compatibility	Units	
PS IMPA	57796	□		RS/RXS 3.0	1	
	58315	■		SC/SCX 3.25	1	
	57819	■		SC/SCX/RS/RXS/RI* ¹ 3.75	1	
	57820	■		SC/SCX/RS/RXS/RI* ¹ 4.1	1	
	57821	■		SC/SCX/RS/RXS/RI* ¹ 4.5	1	
	57822	■		SC/SCX/RS/RXS/RI* ¹ 5.5	1	

^{*1} New version of the BEGO Semados® RI implants, with Platform Switch Design

^{*2} For torque specifications, see page 124

^{*5} Platform Switch Design

Crown restoration Ø 3.0

Provisional abutment Platform Switch

Description	REF	Colour code	Size	Compatibility	Units
PS ITA Material: Titanium alloy Tool: Insertion tool for implants * ²	57778	□		RS/R SX 3.0	1



Solid abutments titanium Platform Switch

Description	REF	Colour code	Size	Compatibility	Units
PS TiAA angle over plane (type P) or edge (type E) comprising: • PS titanium abutment • prosthesis screw RS/R SX 3.0 • technician screw RS/R SX 3.0 Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver * ²	57797	□	15° P GH 2.5–4	RS/R SX 3.0	1
	57798	□	15° E GH 2.5–4	RS/R SX 3.0	1
PS TiA comprising: • PS titanium abutment • prosthesis screw RS/R SX 3.0 • technician screw RS/R SX 3.0 Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver * ²	57776	□	GH 2.5–4	RS/R SX 3.0	1



Angulated abutment, type P

Type P = angle over plane



Angulated abutment, type E

Type E = angle over edge



Crown and bridge restoration Ø 3.25–5.5

Provisional abutments Platform Switch						
Description	REF	Colour code	Size	Compatibility	Units	
PS PPA	58072			SC/SCX/RS/RXS/RI* ¹	3.25–3.75	1
Solid abutment, plastic for provisional restorations comprising:	58073			SC/SCX/RS/RXS/RI* ¹	4.1	1
• PS plastic abutment	58074			SC/SCX/RS/RXS/RI* ¹	4.5	1
• prosthesis screw Hex 1.25 mm	58075			SC/SCX/RS/RXS/RI* ¹	5.5	1
• technician screw L9						
Material: Polyetheretherketone (PEEK)						
Tool: Hexagon screwdriver 1.25 mm / slot screwdriver						
*2						
PS TPA	58146			SC/SCX/RS/RXS/RI* ¹	3.25–3.75	1
comprising:	58147			SC/SCX/RS/RXS/RI* ¹	4.1	1
• PS plastic abutment	58148			SC/SCX/RS/RXS/RI* ¹	4.5	1
• prosthesis screw Hex 1.25 mm						
• technician screw L9						
Material: Polyetheretherketone (PEEK)						
Tool: Hexagon screwdriver 1.25 mm / slot screwdriver						
*2						
PS TTiA	57854			SC/SCX/RS/RXS/RI* ¹	3.25–3.75	1
comprising:	57855			SC/SCX/RS/RXS/RI* ¹	4.1	1
• provisional PS titanium abutment	57856			SC/SCX/RS/RXS/RI* ¹	4.5	1
• prosthesis screw Sub-Tec ^{Plus}	57857			SC/SCX/RS/RXS/RI* ¹	5.5	1
• technician screw Sub-Tec ^{Plus}						
Material: Titanium alloy						
Tool: Hexagon screwdriver 1.25 mm / slot screwdriver						
*2						
PS TTiA NH	57858			SC/SCX/RS/RXS/RI* ¹	3.25–3.75	1
comprising:	57859			SC/SCX/RS/RXS/RI* ¹	4.1	1
• Provisional PS titanium abutment no Hex	57860			SC/SCX/RS/RXS/RI* ¹	4.5	1
• prosthesis screw Sub-Tec ^{Plus}	57861			SC/SCX/RS/RXS/RI* ¹	5.5	1
• technician screw Sub-Tec ^{Plus}						
Material: Titanium alloy						
Tool: Hexagon screwdriver 1.25 mm / slot screwdriver						
*2						
PS ITA	58076			SC/SCX/RS/RXS/RI* ¹	3.25–3.75	1
Material: Titanium alloy	58077			SC/SCX/RS/RXS/RI* ¹	4.1	1
Tool: Insertion tool	58078			SC/SCX/RS/RXS/RI* ¹	4.5	1
Implants						
*2						

^{*1} New version of the BEGO Semados® RI implants, with Platform Switch Design





^{*2} For torque specifications, see page 124

^{*5} Platform Switch Design

Crown and bridge restoration Ø 3.25–5.5









Ceramic abutments Platform Switch						
Description	REF	Colour code	Size	Compatibility	Units	
PS CA comprising: • PS ceramic abutment • prosthesis screw for ceramic abutment • technician screw Sub-Tec ^{Plus} Material: Zirconium oxide Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	58080			SC/SCX/RS/RXS/RI* ¹	3.25–3.75	1
	58081			SC/SCX/RS/RXS/RI* ¹	4.1	1
	58082			SC/SCX/RS/RXS/RI* ¹	4.5	1
	58083			SC/SCX/RS/RXS/RI* ¹	5.5	1
PS CATi comprising: • ceramic sleeve • adhesive abutment • prosthesis screw Sub-Tec ^{Plus} • technician screw Sub-Tec ^{Plus} Material: Zirconium oxide / titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	58084			SC/SCX/RS/RXS/RI* ¹	3.25–3.75	1
	58085			SC/SCX/RS/RXS/RI* ¹	4.1	1
	58086			SC/SCX/RS/RXS/RI* ¹	4.5	1
	58087			SC/SCX/RS/RXS/RI* ¹	5.5	1



Solid abutments titanium Platform Switch						
Description	REF	Colour code	Size	Compatibility	Units	
PS TiA comprising: • PS titanium abutment, conical • prosthesis screw Sub-Tec ^{Plus} • technician screw Sub-Tec ^{Plus} Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	58088			SC/SCX/RS/RXS/RI* ¹	3.25–3.75	1
	58089			SC/SCX/RS/RXS/RI* ¹	4.1	1
	58090			SC/SCX/RS/RXS/RI* ¹	4.5	1
	58091			SC/SCX/RS/RXS/RI* ¹	5.5	1



Crown and bridge restoration Ø 3.25–5.5

Solid abutments titanium Platform Switch						
Description	REF	Colour code	Size	Compatibility		Units
PS TiA comprising: • PS titanium abutment • prosthesis screw Sub-Tec ^{Plus} • technician screw Sub-Tec ^{Plus} Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver * ²	57846		GH 1–2	SC/SCX/RS/RSX/RI* ¹	3.25–3.75	1
	57847		GH 2.5–4	SC/SCX/RS/RSX/RI* ¹	3.25–3.75	1
	57848		GH 1–2	SC/SCX/RS/RSX/RI* ¹	4.1	1
	57849		GH 2.5–4	SC/SCX/RS/RSX/RI* ¹	4.1	1
	57850		GH 1–2	SC/SCX/RS/RSX/RI* ¹	4.5	1
	57851		GH 2.5–4	SC/SCX/RS/RSX/RI* ¹	4.5	1
	57852		GH 1–2	SC/SCX/RS/RSX/RI* ¹	5.5	1
	57853		GH 2.5–4	SC/SCX/RS/RSX/RI* ¹	5.5	1



Solid abutments titanium Platform Switch						
Description	REF	Colour code	Size	Compatibility		Units
PS TiAA angle over plane (type P) or edge (type E) comprising • PS titanium abutment • prosthesis screw Sub-Tec ^{Plus} • technician screw Sub-Tec ^{Plus} Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver * ²	57889		15° P GH 1–2	SC/SCX/RS/RSX/RI* ¹	3.25–3.75	1
	57890		15° P GH 2.5–4	SC/SCX/RS/RSX/RI* ¹	3.25–3.75	1
	57891		15° E GH 1–2	SC/SCX/RS/RSX/RI* ¹	3.25–3.75	1
	57892		15° E GH 2.5–4	SC/SCX/RS/RSX/RI* ¹	3.25–3.75	1
	57893		15° P GH 1–2	SC/SCX/RS/RSX/RI* ¹	4.1	1
	57894		15° P GH 2.5–4	SC/SCX/RS/RSX/RI* ¹	4.1	1
	57895		15° E GH 1–2	SC/SCX/RS/RSX/RI* ¹	4.1	1
	57896		15° E GH 2.5–4	SC/SCX/RS/RSX/RI* ¹	4.1	1
	57897		15° P GH 1–2	SC/SCX/RS/RSX/RI* ¹	4.5	1
	57898		15° P GH 2.5–4	SC/SCX/RS/RSX/RI* ¹	4.5	1
	57899		15° E GH 1–2	SC/SCX/RS/RSX/RI* ¹	4.5	1
	57900		15° E GH 2.5–4	SC/SCX/RS/RSX/RI* ¹	4.5	1
	57905		15° P GH 1–2	SC/SCX/RS/RSX/RI* ¹	5.5	1
	57906		15° P GH 2.5–4	SC/SCX/RS/RSX/RI* ¹	5.5	1
	57907		15° E GH 1–2	SC/SCX/RS/RSX/RI* ¹	5.5	1
	57908		15° E GH 2.5–4	SC/SCX/RS/RSX/RI* ¹	5.5	1


^{*1} New version of the BEGO Semados® RI implants, with Platform Switch Design

^{*2} For torque specifications, see page 124

^{*5} Platform Switch Design

Crown and bridge restoration Ø 3.25–5.5

Solid abutments titanium Platform Switch

Description	REF	Colour code	Size	Compatibility	Units
PS TiAA angle over plane (type P) or edge (type E) comprising • PS titanium abutment • prosthesis screw Sub-Tec ^{Plus} • technician screw Sub-Tec ^{Plus} Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57909	■ ■ ■	20° P GH 1-2	SC/SCX/RS/RXS/RI* ¹ 3.25–3.75	1
	57910	■ ■ ■	20° P GH 2.5-4	SC/SCX/RS/RXS/RI* ¹ 3.25–3.75	1
	57911	■ ■ ■	20° E GH 1-2	SC/SCX/RS/RXS/RI* ¹ 3.25–3.75	1
	57912	■ ■ ■	20° E GH 2.5-4	SC/SCX/RS/RXS/RI* ¹ 3.25–3.75	1
	57913	■ ■ ■	20° P GH 1-2	SC/SCX/RS/RXS/RI* ¹ 4.1	1
	57914	■ ■ ■	20° P GH 2.5-4	SC/SCX/RS/RXS/RI* ¹ 4.1	1
	57915	■ ■ ■	20° E GH 1-2	SC/SCX/RS/RXS/RI* ¹ 4.1	1
	57916	■ ■ ■	20° E GH 2.5-4	SC/SCX/RS/RXS/RI* ¹ 4.1	1
	57917	■ ■ ■	20° P GH 1-2	SC/SCX/RS/RXS/RI* ¹ 4.5	1
	57918	■ ■ ■	20° P GH 2.5-4	SC/SCX/RS/RXS/RI* ¹ 4.5	1
	57919	■ ■ ■	20° E GH 1-2	SC/SCX/RS/RXS/RI* ¹ 4.5	1
	57920	■ ■ ■	20° E GH 2.5-4	SC/SCX/RS/RXS/RI* ¹ 4.5	1
	57921	■ ■ ■	20° P GH 1-2	SC/SCX/RS/RXS/RI* ¹ 5.5	1
	57922	■ ■ ■	20° P GH 2.5-4	SC/SCX/RS/RXS/RI* ¹ 5.5	1
	57923	■ ■ ■	20° E GH 1-2	SC/SCX/RS/RXS/RI* ¹ 5.5	1
	57924	■ ■ ■	20° E GH 2.5-4	SC/SCX/RS/RXS/RI* ¹ 5.5	1



Angulated abutment, type P

Type P = angle over plane



Angulated abutment, type E

Type E = angle over edge










Assortment set Platform Switch

Description	REF	Colour code	Size	Compatibility	Units
PS AS For selecting the correct abutment with corresponding gingival height and angle, comprising: • 20 parts + forceps	58247		0°/15°/20°	SC/SCX/RS/RXS/RI* ¹	1



Crown and bridge restoration Ø 3.25–5.5

Universal abutments Platform Switch						
Description	REF	Colour code	Size	Compatibility	Units	
PS UNI comprising:	57831			SC/SCX/RS/RXS/RI* ¹	3.25–3.75	1
• PS Universal base Hex	57832			SC/SCX/RS/RXS/RI* ¹	4.1	1
• wax-up sleeve Universal	57833			SC/SCX/RS/RXS/RI* ¹	4.5	1
• PS UNI PScrew	57834			SC/SCX/RS/RXS/RI* ¹	5.5	1
• PS UNI TScrew (black)						
Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver * ²						
PS UNI NH comprising:	57835			SC/SCX/RS/RXS/RI* ¹	3.25–3.75	1
• PS Universal base Hex	57836			SC/SCX/RS/RXS/RI* ¹	4.1	1
• wax-up sleeve Universal	57837			SC/SCX/RS/RXS/RI* ¹	4.5	1
• PS UNI PScrew	57838			SC/SCX/RS/RXS/RI* ¹	5.5	1
• PS UNI TScrew (black)						
Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver * ²						
Internal reamer Universal For re-working the internal form fit	55536			S/SC/SCX/RS/RXS/RI	3.25–5.5	1
External reamer Universal For re-working the external form fit	55537			S/SC/SCX/RS/RXS/RI	3.25–5.5	1










*¹ New version of the BEGO Semados® RI implants, with Platform Switch Design

*² For torque specifications, see page 124

*³ Alloy recommendation Bio PontoStar® XL (BEGO, REF 61140)/Bio PontoStar® (BEGO, REF 61104)





*⁵ Platform Switch Design







Crown and bridge restoration Ø 3.25–5.5

Gold cast-on abutments Platform Switch						
Description	REF	Colour code	Size	Compatibility	Units	
PS GCO comprising: • PS cast-on abutment • wax-up sleeve for gold cast-on • prosthesis screw Hex 1.25 mm • technician screw L9 Material: Gold/platinum alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2 *3	58092			SC/SCX/RS/RX/RI* ¹	3.25–3.75	1
	58093			SC/SCX/RS/RX/RI* ¹	4.1	1
	58094			SC/SCX/RS/RX/RI* ¹	4.5	1
	58095			SC/SCX/RS/RX/RI* ¹	5.5	1
PS GCO NH comprising: • PS cast-on abutment no Hex • wax-up sleeve for gold cast-on • prosthesis screw Hex 1.25 mm • technician screw L9 Material: Gold/platinum alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2 *3	58096			SC/SCX/RS/RX/RI* ¹	3.25–3.75	1
	58097			SC/SCX/RS/RX/RI* ¹	4.1	1
	58098			SC/SCX/RS/RX/RI* ¹	4.5	1
	58099			SC/SCX/RS/RX/RI* ¹	5.5	1
Internal reamer for gold cast-on abutment For re-working the internal form fit (a technician screwdriver is recommended as the hold)	53735			S/SC/SCX/RS/RX/RI	3.25–5.5	1



Multi^{Plus} restoration

Auxiliary parts					
Description	REF	Colour code	Size	Compatibility	Units
Multi^{Plus} insertion splint To determine the planned angle	57532			Multi ^{Plus} System	1
Multi^{Plus} bone shaper (Optional) for angled implant bed preparation	57551			S / SC / SCX 3.25	1
	57541			S / SC / SCX 3.75	1
	57542			S / SC / SCX 4.1	1
	57543			S / SC / SCX 4.5	1
Multi^{Plus} alignment aids For aligning the implant hex	57530		20°	Multi ^{Plus} System	1
	57531		30°	Multi ^{Plus} System	1






Multi ^{Plus} abutments Platform Switch					
Description	REF	Colour code	Size	Compatibility	Units
PS Multi^{Plus} comprising: • PS abutment 0° • Multi ^{Plus} positioning aid 0° Material: Titanium alloy (packaged sterile) Tool: Insertion instrument Multi ^{Plus} abutment 0° *2	58100		0° GH 1	SC/SCX/RS/R SX/RI* ¹ 3.25–3.75	1
	58101		0° GH 3	SC/SCX/RS/R SX/RI* ¹ 3.25–3.75	1
	58102		0° GH 1	SC/SCX/RS/R SX/RI* ¹ 4.1	1
	58103		0° GH 3	SC/SCX/RS/R SX/RI* ¹ 4.1	1
	58104		0° GH 1	SC/SCX/RS/R SX/RI* ¹ 4.5	1
	58105		0° GH 3	SC/SCX/RS/R SX/RI* ¹ 4.5	1
Insertion instrument Multi^{Plus} Abutment 0° with ratchet connection	57533			Multi ^{Plus} System	1



*¹ New version of the BEGO Semados® RI implants, with Platform Switch Design

*² For torque specifications, see page 124

*⁵ Platform Switch Design

MultiPlus restoration

MultiPlus abutments Platform Switch						
Description	REF	Colour code	Size	Compatibility	Units	
PS MultiPlus comprising: • PS MultiPlus abutment 20° • MultiPlus positioning aid 20° • prosthesis screw MultiPlus Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	58108		20° GH 2.3–0.6	SC/SCX/RS/RXS/RI* ¹ 3.25–3.75	1	
	58109		20° GH 4.0–2.3	SC/SCX/RS/RXS/RI* ¹ 3.25–3.75	1	
	58110		20° GH 2.3–0.6	SC/SCX/RS/RXS/RI* ¹ 4.1	1	
	58111		20° GH 4.0–2.3	SC/SCX/RS/RXS/RI* ¹ 4.1	1	
	58112		20° GH 2.3–0.6	SC/SCX/RS/RXS/RI* ¹ 4.5	1	
	58113		20° GH 4.0–2.3	SC/SCX/RS/RXS/RI* ¹ 4.5	1	
PS MultiPlus comprising: • PS MultiPlus abutment 30° • MultiPlus positioning aid 30° • prosthesis screw MultiPlus Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	58116		30° GH 4.0–1.5	SC/SCX/RS/RXS/RI* ¹ 3.25–3.75	1	
	58117		30° GH 4.0–1.5	SC/SCX/RS/RXS/RI* ¹ 4.1	1	
	58118		30° GH 4.0–1.5	SC/SCX/RS/RXS/RI* ¹ 4.5	1	

Healing caps						
Description	REF	Colour code	Size	Compatibility	Units	
MultiPlus healing cap Prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm	57520		L5	MultiPlus System	1	
MultiPlus healing cap Mushroom prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm	57521		L5	MultiPlus System	1	

Multi^{Plus} restoration

CAD positioner					
Description	REF	Colour code	Size	Compatibility	Units
CADP Multi^{Plus} • CAD positioner Multi ^{Plus} • secondary screw Multi ^{Plus} Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25 mm *2	58255			Multi ^{Plus} System	1



Impression sets					
Description	REF	Colour code	Size	Compatibility	Units
Multi^{Plus} closed tray impression impression taking on Multi ^{Plus} abutments on closed tray comprising: • Multi ^{Plus} impression post Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm *2	57522		L8	Multi ^{Plus} System	1
	57554		L12	Multi ^{Plus} System	1
Multi^{Plus} open tray impression impression taking on Multi ^{Plus} abutments with open tray comprising: • Multi ^{Plus} impression post • titanium screw L11 and L16 Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm *2	57523		L8	Multi ^{Plus} System	1



Implant analogs					
Description	REF	Colour code	Size	Compatibility	Units
Multi^{Plus} implant analogs	57524			Multi ^{Plus} System	1
	57525			Multi ^{Plus} System	4



*¹ New version of the BEGO Semados® RI implants, with Platform Switch Design

*² For torque specifications, see page 124

*⁵ Platform Switch Design

MultiPlus restoration

MultiPlus titanium abutment					
Description	REF	Colour code	Size	Compatibility	Units
MultiPlus titanium abutment comprising: MultiPlus titanium abutment • secondary screw MultiPlus • technician screw MultiPlus Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57526		L11	MultiPlus System	1






MultiPlus Easy-Con abutment					
Description	REF	Colour code	Size	Compatibility	Units
MultiPlus MC Material: Titanium alloy with TiN coating Tool: Insertion tool ³ Locator® *2	58240			MultiPlus System	2





Protection analog					
Description	REF	Colour code	Size	Compatibility	Units
MultiPlus protection analog To protect the basal margins when finishing the prosthesis Material: Titanium alloy	57537			MultiPlus System	4



Multi^{Plus} restoration

Multi ^{Plus} Universal abutment					
Description	REF	Colour code	Size	Compatibility	Units
Multi^{Plus} Universal comprising: <ul style="list-style-type: none"> • Multi^{Plus} wax-up sleeve Universal • secondary screw Multi^{Plus} • technician screw Multi^{Plus} Material: Polyoxymethylene (POM) Tool: Hexagon screwdriver 1.25 mm / slot screwdriver * ²	57538		L11	Multi ^{Plus} System	1
					
Multi^{Plus} internal reamer For re-working the internal form fit including reamer handle	57540			Multi ^{Plus} System	1
					
Multi^{Plus} external reamer For re-working the external form fit including reamer handle	57539			Multi ^{Plus} System	1
					

Multi ^{Plus} gold cast-on abutment					
Description	REF	Colour code	Size	Compatibility	Units
Multi^{Plus} gold cast-on comprising: <ul style="list-style-type: none"> • Multi^{Plus} cast-on abutment • Multi^{Plus} wax-up sleeve gold cast-on • secondary screw Multi^{Plus} • technician screw Multi^{Plus} Material: Gold/platinum alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver * ² * ³	57527			Multi ^{Plus} System	1
					
Multi^{Plus} internal reamer For re-working the internal form fit including reamer handle	57540			Multi ^{Plus} System	1
					

Note: For manufacturer's information on trademarks, see page 122.










*¹ New version of the BEGO Semados® RI implants, with Platform Switch Design

*² For torque specifications, see page 124

*³ Alloy recommendation Bio PontoStar® XL (BEGO, REF 61140)/Bio PontoStar® (BEGO, REF 61104)

*⁵ Platform Switch Design

Hybrid restoration Ø3.25–4.5

Ball attachment abutments Platform Switch						
Description	REF	Colour code	Size	Compatibility		Units
PS BA comprising: • PS ball attachment with no female part • distance spacer Material: Titanium alloy Tool: Insertion tool Ball attachment * ²	58120		GH 0	SC/SCX/RS/RX/RI* ¹	3.25–3.75	1
	58121		GH 3	SC/SCX/RS/RX/RI* ¹	3.25–3.75	1
	58122		GH 5	SC/SCX/RS/RX/RI* ¹	3.25–3.75	1
	58123		GH 0	SC/SCX/RS/RX/RI* ¹	4.1	1
	58124		GH 3	SC/SCX/RS/RX/RI* ¹	4.1	1
	58125		GH 5	SC/SCX/RS/RX/RI* ¹	4.1	1
	58126		GH 0	SC/SCX/RS/RX/RI* ¹	4.5	1
	58127		GH 3	SC/SCX/RS/RX/RI* ¹	4.5	1
	58128		GH 5	SC/SCX/RS/RX/RI* ¹	4.5	1
Insertion tool for ball attachment with ratchet connection	55880					1

















Ball attachment impression set ² Dalbo®						
Description	REF	Colour code	Size	Compatibility		Units
Ball attachment impression set ²Dalbo®-PLUS impression on ball attachment comprising: • impression cap for ball attachment (red) • implant analog for ball attachment	55768					1



Ball attachment female parts ² Dalbo®						
Description	REF	Colour code	Size	Compatibility		Units
Female parts ²Dalbo®-PLUS comprising: • female parts ² Dalbo®-PLUS, complete (incl. retention insert) • placeholder Material: Titanium grade 4 Tool: ² Dalbo®-PLUS activator/deactivator	55769					1
²Dalbo®-PLUS activator/deactivator	55773					1
Retention insert ²Dalbo®-PLUS Material: Precious metal Tool: ² Dalbo®-PLUS activator/deactivator	55776					1



Hybrid restoration Ø 3.75–4.5

Easy-Con abutments Platform Switch						
Description	REF	Colour code	Size	Compatibility		Units
PS Easy-Con Material: Titanium alloy with TiN coating Tool: Insertion tool ³ Locator® * ²	58130		L1	SC/SCX/RS/RX/RI* ¹	3.75	1
	58131		L2	SC/SCX/RS/RX/RI* ¹	3.75	1
	58132		L3	SC/SCX/RS/RX/RI* ¹	3.75	1
	58133		L4	SC/SCX/RS/RX/RI* ¹	3.75	1
	58134		L1	SC/SCX/RS/RX/RI* ¹	4.1	1
	58135		L2	SC/SCX/RS/RX/RI* ¹	4.1	1
	58136		L3	SC/SCX/RS/RX/RI* ¹	4.1	1
	58137		L4	SC/SCX/RS/RX/RI* ¹	4.1	1
	58138		L1	SC/SCX/RS/RX/RI* ¹	4.5	1
	58139		L2	SC/SCX/RS/RX/RI* ¹	4.5	1
	58140		L3	SC/SCX/RS/RX/RI* ¹	4.5	1
	58141		L4	SC/SCX/RS/RX/RI* ¹	4.5	1
	58142		L2	SC/SCX/RS/RX/RI* ¹	5.5	1
	58143		L4	SC/SCX/RS/RX/RI* ¹	5.5	1
Insertion tool ³Locator® with ratchet connection (also for Easy-Con)	57008					1



Easy-Con impression						
Description	REF	Colour code	Size	Compatibility		Units
Easy-Con impression coping Impression on Easy-Con	57751					4
Easy-Con analog	57760					4



Note: For manufacturer's information on trademarks, see page 122.

*¹ New version of the BEGO Semados® RI implants, with Platform Switch Design






*² For torque specifications, see page 124

*⁵ Platform Switch Design

Hybrid restoration Ø3.75–4.5

Easy-Con female parts					
Description	REF	Colour code	Size	Compatibility	Units
Easy-Con laboratory set comprising: • retention insert transparent, pink and blue • block-out ring • retention cap • fabrication insert, black Material: Titanium alloy / polyamide (PA12) Tool: Easy-Con instrument	57752				2
Easy-Con instrument For screw-fitting, removing and repositioning the retention inserts, insertion aid for Easy-Con abutment	57753				1
Easy-Con fabrication insert (black) Material: Polyamide (PA12)	57754				4
Easy-Con retention insert (blue) Withdrawal force: 680 g; 6.7 N; 0–10° Material: Polyamide (PA12)	57755				4
Easy-Con retention insert (pink) Withdrawal force: 1361 g; 13.4 N; 0–10° Material: Polyamide (PA12)	57756				4
Easy-Con retention insert (transparent) Withdrawal force: 2268 g; 22.3 N; 0–10° Material: Polyamide (PA12)	57757				4
Easy-Con retention insert (red) Withdrawal force: 680 g; 6.7 N; 10–20° Material: Polyamide (PA12)	57758				4
Easy-Con retention insert (green) Withdrawal force: 1814 g; 17.8 N; 10–20° Material: Polyamide (PA12)	57759				4

Hybrid restoration Ø 3.25–4.5

Bar abutments Platform Switch						
Description	REF	Colour code	Size	Compatibility	Units	
² DOLDER® bar joint attachment 3.0 – titanium Material: Titanium grade 4	55928		L50		1	
PS TiBA comprising:	58155			SC/SCX/RS/RX/RI* ¹	3.25–3.75	
• titanium bar abutment	58156			SC/SCX/RS/RX/RI* ¹	4.1	
• prosthesis screw Sub-Tec ^{Plus}	58157			SC/SCX/RS/RX/RI* ¹	4.5	
• technician screw Sub-Tec ^{Plus} Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25 mm / slot screwdriver * ²						





Note: For manufacturer's information on trademarks, see page 122.

*¹ New version of the BEGO Semados® RI implants, with Platform Switch Design








*² For torque specifications, see page 124

*⁵ Platform Switch Design

Screws

Technician screws					
Description	REF	Colour code	Size	Compatibility	Units
Technician screw L9	53762			PS PPA, PS TPA, PS GCO/PS GCO NH	1
Technician screw Sub-Tec ^{Plus}	57028			PS CA, PS CATi, PS PMB, PS TiB/PS TiB NH, PS TTiA/PS TTiA NH, PS TiAA, PS TiA, PS TiBA	1
Technician screw Multi ^{Plus} (M1.4)	57536			Multi ^{Plus} System	1
TScrew	57783			Platform Switch Prosthetics Ø 3.0	1
PS UNI TScrew	57994			PS UNI/PS UNI NH	1

Screws

Prosthesis screws					
Description	REF	Colour code	Size	Compatibility	Units
Prosthesis screw Hex 1.25 mm	53999			Healing posts individual Ø 7, PS CADP, PS PPA, PS TPA, PS GCO/PS GCO NH	1
Prosthesis screw for ceramic abutment	56094			PS CA	1
Prosthesis screw Sub-Tec ^{Plus}	57031			CAD SP, PS CATi, PS OCP, PS PMB, PS TiB/PS TiB NH, PS TTiA/PS TTiA NH, PS TiAA, PS TiA, PS TiBA	1
Secondary screw Multi ^{Plus} (M1.4)	57534			Multi ^{Plus} System	1
Prosthesis screw Multi ^{Plus} (M1.8)	57535			PS Multi ^{Plus} 20/30°	1
PScrew	57782			Platform Switch Prosthetics Ø 3.0	1
PScrew	57784			CAD positioner Platform Switch Ø 3.0	1
PS UNI PScrew	57993			PS UNI/PS UNI NH	1

*¹ New version of the BEGO Semados® RI implants, with Platform Switch Design

*⁵ Platform Switch Design



OVERVIEW

CAD/CAM restoration	92
Impression taking and model fabrication	92
Crown restoration	93
Hybrid restoration	94
Screws	97

CAD/CAM restoration

CAD positioner					
Description	REF	Colour code	Size	Compatibility	Units
CADP comprising: • CAD positioner Mini • prosthesis screw Mini Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25 mm *2	58256	■		Mini 2.7–3.1	1



Impression taking and model fabrication

Impression set					
Description	REF	Colour code	Size	Compatibility	Units
Open tray impression Mini impression on implant with open tray technique comprising: • Mini impression posts • titanium screw L15 and L19 Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	56959	■		Mini 2.7–3.1	1



Implant analog					
Description	REF	Colour code	Size	Compatibility	Units
Model implant Mini	56982	■		Mini 2.7–3.1	1



*2 For torque specifications, see page 124

*3 Alloy recommendation: Bio PontoStar® XL (BEGO, REF 61140)/Bio PontoStar® (BEGO, REF 61104)

Crown restoration

Solid abutment titanium

Description	REF	Colour code	Size	Compatibility	Units
TiA comprising: <ul style="list-style-type: none"> • titanium Mini abutment • prosthesis screw Mini • technician screw Mini Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57989	■		Mini 2.9–3.1	1




Gold cast-on abutment

Description	REF	Colour code	Size	Compatibility	Units
Gold cast-on Mini comprising: <ul style="list-style-type: none"> • cast-on abutment Mini • sub wax-up sleeve gold cast-on • prosthesis screw Mini, conical • technician screw Mini, conical Material: Gold/platinum alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2 *3	57320	■		Mini 2.9–3.1	1
Internal reamer for gold cast-on Mini for re-working the internal form fit (a technician screwdriver is recommended as the hold)	57323	■		Mini-Line	1



Hybrid restoration

Bar abutments					
Description	REF	Colour code	Size	Compatibility	Units
²DOLDER® bar joint attachment 3.0 – titanium Material: Titanium grade 4	55928		L50		1
TiBA comprising: • titanium bar abutment Mini • prosthesis screw Mini • technician screw Mini Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57988	■		Mini 2.7–3.1	1



Easy-Con abutments					
Description	REF	Colour code	Size	Compatibility	Units
Easy-Con Mini Material: Titanium alloy with TiN coating Tool: Insertion tool ³ Locator® *2	57623	■	L1.5	Mini 3.1	1
	57624	■	L2.5	Mini 3.1	1
	57625	■	L3.5	Mini 3.1	1
Insertion tool ³Locator® with ratchet connection (also for Easy-Con)	57008				1



Easy-Con impression					
Description	REF	Colour code	Size	Compatibility	Units
Easy-Con impression coping (impression on Easy-Con)	57751				4
Easy-Con analog	57760				4





Note: For manufacturer's information on trademarks, see page 122.


*2 For torque specifications, see page 124




Hybrid restoration

Easy-Con female parts					
Description	REF	Colour code	Size	Compatibility	Units
Easy-Con laboratory set comprising: • retention insert transparent, pink and blue • block-out ring • retention cap • fabrication insert, black Material: Titanium alloy / polyamide (PA12) Tool: Easy-Con instrument	57752				2
Easy-Con instrument for screw-fitting, removing and repositioning the retention inserts, insertion aid for Easy-Con abutment	57753				1
Easy-Con fabrication insert (black) Material: Polyamide (PA12)	57754				4
Easy-Con retention insert (blue) Withdrawal force: 680 g; 6.7 N; 0–10° Material: Polyamide (PA12)	57755				4
Easy-Con retention insert (pink) Withdrawal force: 1361 g; 13.4 N; 0–10° Material: Polyamide (PA12)	57756				4
Easy-Con retention insert (transparent) Withdrawal force: 2268 g; 22.3 N; 0–10° Material: Polyamide (PA12)	57757				4
Easy-Con retention insert (red) Withdrawal force: 680 g; 6.7 N; 10–20° Material: Polyamide (PA12)	57758				4
Easy-Con retention insert (green) Withdrawal force: 1814 g; 17.8 N; 10–20° Material: Polyamide (PA12)	57759				4

Hybrid restoration

Ball attachment abutments						
Description	REF	Colour code	Size	Compatibility		Units
Ball attachment Mini Material: Titanium alloy Tool: Insertion tool Ball attachment *2	56968	■	GH 1.5	Mini 2.9–3.1		1
	57055	■	GH 4	Mini 2.9–3.1		1
						
Insertion tool for ball attachment with ratchet connection	55880					1 

Ball attachment impression set ² Dalbo®						
Description	REF	Colour code	Size	Compatibility		Units
Ball attachment impression set ²Dalbo®-PLUS impression on ball attachment comprising: <ul style="list-style-type: none"> • impression cap for ball attachment (red) • implant analog for ball attachment 	55768					1 

Ball attachment female parts ² Dalbo®						
Description	REF	Colour code	Size	Compatibility		Units
Female parts ²Dalbo®-PLUS comprising: <ul style="list-style-type: none"> • female parts ²Dalbo®-PLUS, complete (incl. retention insert) • placeholder Material: Titanium grade 4 Tool: ² Dalbo®-PLUS activator / deactivator	55769					1 
²Dalbo®-PLUS activator / deactivator	55773					1 
Retention insert ²Dalbo®-PLUS Material: Precious metal Tool: ² Dalbo®-PLUS activator / deactivator	55776					1 

Note: For manufacturer's information on trademarks, see page 122.

*2 For torque specifications, see page 124


Screws

Technician screws					
Description	REF	Colour code	Size	Compatibility	Units
Technician screw Mini	56984	■		TiA, TiBA	1
Technician screw Mini, conical	57322	■		Gold cast-on Mini	1



Prosthesis screws					
Description	REF	Colour code	Size	Compatibility	Units
Prosthesis screw Mini	56983	■		TiA, TiBA, CADP (Mini)	1
Prosthesis screw Mini, conical	57321	■		Gold cast-on Mini	1



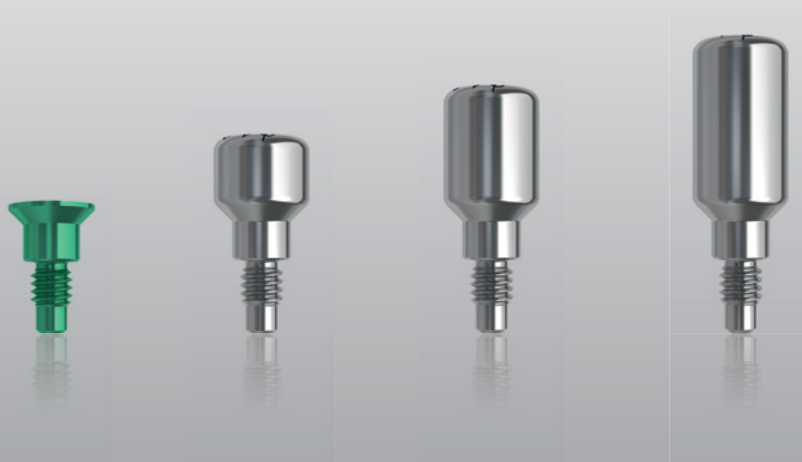




























OVERVIEW

Cover screws
Healing posts

100


100

Cover screws						
Description	REF	Colour code	Size	Compatibility	Units	
Implant	55505			S 3.25	1	
cover screw	55608			S / RI 3.75	1	
Material: Titanium grade 4 (packaged sterile)	55615			S / RI 4.1	1	
Tool: Hexagon screwdriver 1.25 mm	55616			S / RI 4.5	1	
*2	55908			S / RI 5.5	1	

Healing posts						
Description	REF	Colour code	Size	Compatibility	Units	
Healing posts prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	Healing posts Ø4.0					
	55590		L3	S / RI 3.25–3.75	1	
	55591		L5	S / RI 3.25–3.75	1	
	55592		L7	S / RI 3.25–3.75	1	
	Healing posts Ø4.5					
	56300		L3	S / RI 3.25–4.5	1	
	56301		L5	S / RI 3.25–4.5	1	
	56302		L7	S / RI 3.25–4.5	1	
	Healing posts Ø5.0					
	55593		L3	S / RI 3.25–4.5	1	
	55594		L5	S / RI 3.25–4.5	1	
	55595		L7	S / RI 3.25–4.5	1	
	Healing posts Ø6.0					
	56303		L3	S / RI 3.25–5.5	1	
	56304		L5	S / RI 3.25–5.5	1	
	56305		L7	S / RI 3.25–5.5	1	
Healing posts, conical pefabricated gingival former for bar restorations Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	Healing posts Ø6.0					
	57324		L5	S / RI 3.25–3.75	1	
	57339		L5	S / RI 4.1	1	
Healing posts, individual customisable gingival former comprising: • healing post • prosthesis screw Hex 1.25 mm Material: Polyetheretherketone (PEEK) Tool: Hexagon screwdriver 1.25 mm *2	55953		Ø 7.0	S / SC/SCX/RS/R SX/RI 3.25–5.5	1	

*2 For torque specifications, see page 124

*5 Platform Switch Design

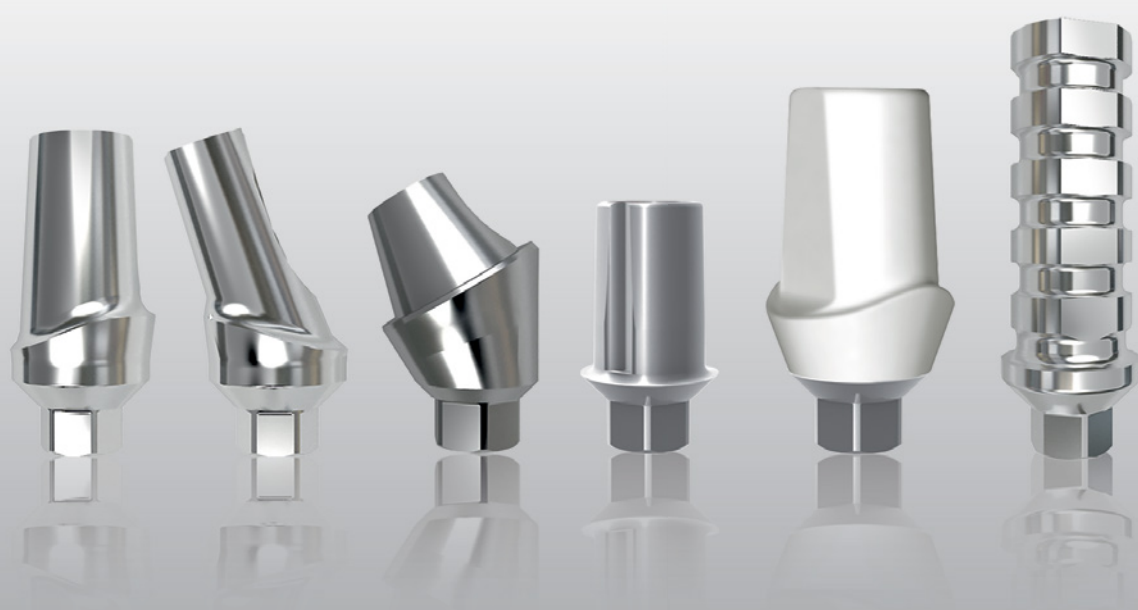













OVERVIEW

CAD/CAM restoration	102
Impression taking and model fabrication	104
Crown and bridge restoration	105
Multi ⁱ Plus restoration	110
Hybrid restoration	115
Screws	118

Note: The entire Platform Switch prosthetic range for SC / SCX / RS / RSX and the new RI implants with Platform Switch Design (CAD/CAM restoration, impression taking and model fabrication, crown and bridge restoration, hybrid restoration) can be found on page 67 onwards of this product catalogue.

CAD/CAM restoration

CAD positioner					
Description	REF	Colour code	Size	Compatibility	Units
Sub-Tec CAD positioner comprising: • Sub-Tec CAD positioner • prosthesis screw Hex 1.25 mm Material: Titan Grade 4 Tool: Hexagon screwdriver 1.25 mm *2	57060			S / RI 3.25–5.5	1
					
Adhesive abutments					
Description	REF	Colour code	Size	Compatibility	Units
Sub-Tec CAD/CAM titanium adhesive abutment comprising: • Sub-Tec adhesive abutment • prosthesis screw Sub-Tec ^{Plus} • technician screw Sub-Tec ^{Plus} Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57285			S / RI 3.25–5.5	1
	57287			S / RI 4.1	1
	57289			S / RI 4.5	1
	57291			S / RI 5.5	1
					
Sub-Tec CAD/CAM titanium adhesive abutment no Hex comprising: • Sub-Tec adhesive abutment no Hex • prosthesis screw Sub-Tec ^{Plus} • technician screw Sub-Tec ^{Plus} Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57286			S / RI 3.25–3.75	1
	57288			S / RI 4.1	1
	57290			S / RI 4.5	1
	57292			S / RI 5.5	1
					






*1 New version of the BEGO Semados® RI implants, with Platform Switch Design






*2 For torque specifications, see page 124




*5 Platform Switch Design

*6 This symbol is a commercial name / registered trademark of a business that does not belong to the BEGO Group.

CAD/CAM restoration

Adhesive abutments						
Description	REF	Colour code	Size	Compatibility	Units	
Sub-Tec CAD/CAM TiBase L	57656			S / RI 3.25–3.75	1	
comprising:						
• Sub-Tec TiBase	57657			S / RI 4.1	1	
• prosthesis screw Sub-Tec ^{plus}	57658			S / RI 4.5	1	
• technician screw Sub-Tec ^{plus}	57659			S / RI 5.5	1	
Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2						













Scansupport						
Description	REF	Colour code	Size	Compatibility	Units	
CAD SP	58191			S / SC / SCX / RS / RSX / RI 3.25–3.75	1	
comprising:						
• scansupport	58192			S / SC / SCX / RS / RSX / RI 4.1	1	
• prosthesis screw Sub-Tec ^{plus}	58193			S / SC / SCX / RS / RSX / RI 4.5	1	
Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm *2	58194			S / SC / SCX / RS / RSX / RI 5.5	1	







CAD/CAM milling blank						
Description	REF	Colour code	Size	Compatibility	Units	
ST PMB	58319		Ø 11.5	S / RI 3.25–5.5	1	
comprising:						
comprising:	58219		Ø 16	S / RI 3.25–5.5	1	
• milling blank:						
• prosthesis screw Sub-Tec ^{plus}						
• technician screw Sub-Tec ^{plus}						
Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm, slot screwdriver *2						

Note: When using the *6Cerec® system a *6Cerec/*6InLab Scanbody for *6Bluecam (36 units) REF 6431303 or Scanbody for *6Omnicam (36 units) REF 6431329 (Sirona Dental Systems GmbH, Bensheim, Germany) is required.

Note: A *6PreFace® abutment holder is required for the corresponding milling machine. This must be ordered directly from the machine manufacturer. You must follow the manufacturer's instructions.

Impression taking and model fabrication

Impression sets						
Description	REF	Colour code	Size	Compatibility	Units	
Sub-Dent closed tray impression impression taking on implant with closed tray comprising: <ul style="list-style-type: none"> • impression post cap • sub impression post • titanium screw L11 Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	55860			S 3.25	1	
	55539			S / RI 3.75	1	
	55617			S / RI 4.1	1	
	55618			S / RI 4.5	1	
	55551			S / RI 5.5	1	
Sub-Dent open tray impression impression taking on implant with open tray comprising: <ul style="list-style-type: none"> • sub impression post • titanium screw L16 and L21 Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	55861			S 3.25	1	
	55540			S / RI 3.75	1	
	55619			S / RI 4.1	1	
	55620			S / RI 4.5	1	
	56500			S / RI 5.5	1	

Implant analogs						
Description	REF	Colour code	Size	Compatibility	Units	
Model implants	56694			S 3.25	1	
	56695			S / RI 3.75	1	
	56696			S / RI 4.1	1	
	56698			S / RI 4.5	1	
	56699			S / RI 5.5	1	

*2 For torque specifications, see page 124

*5 Platform Switch Design

Crown and bridge restoration

Provisional abutments						
Description	REF	Colour code	Size	Compatibility	Units	
Sub-Tec provisional abutment solid abutment, plastic for provisional restorations comprising: <ul style="list-style-type: none"> • plastic abutment • prosthesis screw Hex 1.25 mm • technician screw L9 Material: Polyetheretherketone (PEEK) Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	55951		Ø 7	S / RI 3.25–5.5	1	
Sub-Tec provisional PEEK abutment comprising: <ul style="list-style-type: none"> • plastic abutment • prosthesis screw Hex 1.25 mm • technician screw L9 Material: Polyetheretherketone (PEEK) Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57494			S / RI 3.25–3.75	1	
	57495			S / RI 4.1–4.5	1	
Sub-Tec provisional titanium abutment comprising: <ul style="list-style-type: none"> • sub-Tec provisional titanium abutment • prosthesis screw Sub-Tec^{plus} • technician screw Sub-Tec^{plus} Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57304			S / RI 3.25–3.75	1	
	57305			S / RI 4.1	1	
	57306			S / RI 4.5	1	
	57307			S / RI 5.5	1	
Sub-Tec provisional titanium abutment no Hex comprising: <ul style="list-style-type: none"> • Sub-Tec provisional titanium abutment no Hex • prosthesis screw Sub-Tec^{plus} • technician screw Sub-Tec^{plus} Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57300			S / RI 3.25–3.75	1	
	57301			S / RI 4.1	1	
	57302			S / RI 4.5	1	
	57303			S / RI 5.5	1	

Crown and bridge restoration

Ceramic abutments					
Description	REF	Colour code	Size	Compatibility	Units
BeCe® Sub-Tec ceramic abutment comprising: • ceramic abutment • prosthesis screw for ceramic abutment • technician screw Sub-Tec ^{Plus} Material: Zirconium oxide Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	56092			S / RI 3.25–5.5	1
BeCe® Sub-Tec ceramic abutment comprising: • ceramic sleeve • adhesive abutment • prosthesis screw Sub-Tec ^{Plus} • technician screw Sub-Tec ^{Plus} Material: Zirconium oxide / titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57680			S / RI 3.25–3.75	1
	57681			S / RI 4.1	1
	57682			S / RI 4.5	1
	57683			S / RI 5.5	1



Solid abutments titanium					
Description	REF	Colour code	Size	Compatibility	Units
Sub-Tec^{Plus} titanium abutment comprising: • titanium abutment • prosthesis screw Sub-Tec ^{Plus} • technician screw Sub-Tec ^{Plus} Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57116		GH 1-2	S / RI 3.25–3.75	1
	57117		GH 2.5–4	S / RI 3.25–3.75	1
	57120		GH 1-2	S / RI 4.1	1
	57121		GH 2.5–4	S / RI 4.1	1
	57124		GH 1-2	S / RI 4.5	1
	57125		GH 2.5–4	S / RI 4.5	1
	57128		GH 1-2	S / RI 5.5	1
	57129		GH 2.5–4	S / RI 5.5	1



*2 For torque specifications, see page 124

*5 Platform Switch Design

Crown and bridge restoration

Solid abutments titanium						
Description	REF	Colour code	Size	Compatibility	Units	
Sub-Tec^{Plus} titanium angulated abutment angle over plane (type P) or edge (type E) comprising <ul style="list-style-type: none"> • angulated abutment • prosthesis screw Sub-Tec^{Plus} • technician screw Sub-Tec^{Plus} Material: Titanium alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57132		15° P GH 1-2	S / RI 3.25-3.75	1	
	57133		15° P GH 2.5-4	S / RI 3.25-3.75	1	
	57134		15° E GH 1-2	S / RI 3.25-3.75	1	
	57135		15° E GH 2.5-4	S / RI 3.25-3.75	1	
	57136		15° P GH 1-2	S / RI 4.1	1	
	57137		15° P GH 2.5-4	S / RI 4.1	1	
	57138		15° E GH 1-2	S / RI 4.1	1	
	57139		15° E GH 2.5-4	S / RI 4.1	1	
	57140		15° P GH 1-2	S / RI 4.5	1	
	57141		15° P GH 2.5-4	S / RI 4.5	1	
	57142		15° E GH 1-2	S / RI 4.5	1	
	57143		15° E GH 2.5-4	S / RI 4.5	1	
	57144		15° P GH 1-2	S / RI 5.5	1	
	57145		15° P GH 2.5-4	S / RI 5.5	1	
	57146		15° E GH 1-2	S / RI 5.5	1	
	57147		15° E GH 2.5-4	S / RI 5.5	1	



PROSTHETICS · WITHOUT PS*5 DESIGN

Angulated abutment, type P

Type P = angle over plane













Angulated abutment, type E

Type E = angle over edge



Crown and bridge restoration










Universal abutments						
Description	REF	Colour code	Size	Compatibility	Units	
Sub-Tec Universal comprising:	55525			S / RI 3.25–3.75	1	
• Universal base Hex	55622			S / RI 4.1	1	
• sub wax-up sleeve Universal	55527			S / RI 4.5	1	
• prosthesis screw						
Sub-Tec Universal	55529			S / RI 5.5	1	
• technician screw						
Sub-Tec Universal (black)						
Material: Titanium alloy						
Tool: Hexagon screwdriver						
1.25 mm / slot screwdriver						
*2						
Sub-Tec Universal no Hex comprising:	55526			S / RI 3.25–3.75	1	
• Universal base no Hex	55623			S / RI 4.1	1	
• sub wax-up sleeve Universal	55528			S / RI 4.5	1	
• prosthesis screw						
Sub-Tec Universal	55530			S / RI 5.5	1	
• technician screw						
Sub-Tec Universal (black)						
Material: Titanium alloy						
Tool: Hexagon screwdriver						
1.25 mm / slot screwdriver						
*2						
Internal reamer Universal for re-working the internal form fit	55536			S / SC / SCX / RS / RSX / RI 3.25–5.5	1	
External reamer Universal for re-working the external form fit	55537			S / SC / SCX / RS / RSX / RI 3.25–5.5	1	

*2 For torque specifications, see page 124

*3 Alloy recommendation: Bio PontoStar® XL (BEGO, REF 61140)/Bio PontoStar® (BEGO, REF 61104)





*5 Platform Switch Design

Crown and bridge restoration







Gold cast-on abutments					
Description	REF	Colour code	Size	Compatibility	Units
Sub-Tec gold cast-on	55862			S / RI 3.25–3.75	1
comprising:					
• sub cast-on abutment	55624			S / RI 4.1	1
• sub wax-up sleeve gold cast-on	56317			S / RI 4.5	1
• prosthesis screw Hex 1.25 mm					
• technician screw L9	56510			S / RI 5.5	1
Material: Gold/platinum alloy					
Tool: Hexagon screwdriver					
1.25 mm / slot screwdriver					
*2 *3					
Sub-Tec gold cast-on no Hex	55873			S / RI 3.25–3.75	1
comprising:					
• sub cast-on abutment no Hex	55625			S / RI 4.1	1
• sub wax-up sleeve gold cast-on	56325			S / RI 4.5	1
• prosthesis screw Hex 1.25 mm					
• technician screw L9	56515			S / RI 5.5	1
Material: Gold/platinum alloy					
Tool: Hexagon screwdriver					
1.25 mm / slot screwdriver					
*2 *3					
Internal reamer for gold cast-on abutment	53735			S / SC / SCX / RS / RSX / RI 3.25–5.5	1
for re-working the internal form fit (a technician screwdriver is recommended as the hold)					



Multi^{Plus} restoration

Auxiliary parts					
Description	REF	Colour code	Size	Compatibility	Units
Multi^{Plus} insertion splint to determine the planned angulation	57532			Multi ^{Plus} System	1
Multi^{Plus} bone shaper (Optional) for angled implant bed preparation	57551			S / SC / SCX 3.25	1
	57541			S / SC / SCX 3.75	1
	57542			S / SC / SCX 4.1	1
	57543			S / SC / SCX 4.5	1
Multi^{Plus} alignment aids for aligning the implant hex	57530		20°	Multi ^{Plus} System	1
	57531		30°	Multi ^{Plus} System	1







Multi ^{Plus} abutments					
Description	REF	Colour code	Size	Compatibility	Units
Sub-Tec Multi^{Plus} abutment comprising: • Sub-Tec Multi ^{Plus} abutment 0° • Multi ^{Plus} positioning aid 0° Material: Titanium alloy (packaged sterile) Tool: Insertion instrument Multi ^{Plus} abutment 0° *2	57505		0° GH 1	S / RI 3.25–3.75	1
	57508		0° GH 3	S / RI 3.25–3.75	1
	57506		0° GH 1	S / RI 4.1	1
	57509		0° GH 3	S / RI 4.1	1
	57507		0° GH 1	S / RI 4.5	1
	57510		0° GH 3	S / RI 4.5	1
Insertion instrument Multi^{Plus} abutment 0° with ratchet connection	57533			Multi ^{Plus} System	1



*2 For torque specifications, see page 124

*5 Platform Switch Design

MultiPlus restoration

MultiPlus abutments						
Description	REF	Colour code	Size	Compatibility	Units	
Sub-Tec MultiPlus abutment comprising: <ul style="list-style-type: none">• Sub-Tec MultiPlus abutment 20°• MultiPlus positioning aid 20°• prosthesis screw MultiPlus Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57511		20° GH 2.3-0.6	S / RI 3.25–3.75	1	
	57514		20° GH 4.0–2.3	S / RI 3.25–3.75	1	
	57512		20° GH 2.3-0.6	S / RI 4.1	1	
	57515		20° GH 4.0–2.3	S / RI 4.1	1	
	57513		20° GH 2.3-0.6	S / RI 4.5	1	
	57516		20° GH 4.0–2.3	S / RI 4.5	1	
Sub-Tec MultiPlus abutment comprising: <ul style="list-style-type: none">• Sub-Tec MultiPlus abutment 30°• MultiPlus positioning aid 30°• prosthesis screw MultiPlus Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57517		30° GH 4.0-1.5	S / RI 3.25–3.75	1	
	57518		30° GH 4.0-1.5	S / RI 4.1	1	
	57519		30° GH 4.0-1.5	S / RI 4.5	1	
Healing caps						
Description	REF	Colour code	Size	Compatibility	Units	
MultiPlus healing cap prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm	57520		L5	MultiPlus System	1	
MultiPlus healing cap Mushroom prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm	57521		L5	MultiPlus System	1	

Multi^{Plus} restoration

CAD positioner					
Description	REF	Colour code	Size	Compatibility	Units
CADP Multi^{Plus} • CAD positioner Multi ^{Plus} • secondary screw Multi ^{Plus} Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25 mm *2	58255			Multi ^{Plus} System	1



Impression sets					
Description	REF	Colour code	Size	Compatibility	Units
Multi^{Plus} closed tray impression impression taking on Multi ^{Plus} abutments on closed tray comprising: • Multi ^{Plus} impression post Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm *2	57522		L8	Multi ^{Plus} System	1
impression taking on Multi ^{Plus} abutments on closed tray comprising: • Multi ^{Plus} impression post Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm *2	57554		L12	Multi ^{Plus} System	1
Multi^{Plus} open tray impression (impression taking on Multi ^{Plus} abutments with open tray) comprising: • Multi ^{Plus} impression post • titanium screw L11 and L16 Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm *2	57523		L8	Multi ^{Plus} System	1



Implant analog					
Description	REF	Colour code	Size	Compatibility	Units
Multi^{Plus} implant analog	57524			Multi ^{Plus} System	1
	57525			Multi ^{Plus} System	4



*2 For torque specifications, see page 124

*5 Platform Switch Design

MultiPlus restoration

MultiPlus titanium abutment					
Description	REF	Colour code	Size	Compatibility	Units
MultiPlus titanium abutment comprising: MultiPlus titanium abutment • secondary screw MultiPlus • technician screw MultiPlus Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57526		L11	MultiPlus System	1



MultiPlus Easy-Con abutment					
Description	REF	Colour code	Size	Compatibility	Units
MultiPlus MC Material: Titanium alloy with TiN coating Tool: Insertion tool ³ Locator® *2	58240			MultiPlus System	2



Protection analog					
Description	REF	Colour code	Size	Compatibility	Units
MultiPlus protection analog to protect the basal margins when finishing the prosthesis Material: Titanium alloy	57537			MultiPlus System	4



MultiPlus restoration

MultiPlus Universal abutment					
Description	REF	Colour code	Size	Compatibility	Units
MultiPlus Universal comprising: <ul style="list-style-type: none"> • MultiPlus wax-up sleeve Universal • secondary screw MultiPlus • technician screw MultiPlus Material: Polyoxymethylene (POM) Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2	57538		L11	MultiPlus System	1
MultiPlus internal reamer for re-working the internal form fit including reamer handle	57540			MultiPlus System	1
MultiPlus external reamer For re-working the external form fit including reamer handle	57539			MultiPlus System	1



MultiPlus gold cast-on abutment					
Description	REF	Colour code	Size	Compatibility	Units
MultiPlus gold cast-on comprising: <ul style="list-style-type: none"> • MultiPlus cast-on abutment • MultiPlus wax-up sleeve gold cast-on • secondary screw MultiPlus • technician screw MultiPlus Material: Gold/platinum alloy Tool: Hexagon screwdriver 1.25 mm / slot screwdriver *2 *3	57527			MultiPlus System	1
MultiPlus internal reamer for re-working the internal form fit including reamer handle	57540			MultiPlus System	1









Note: For manufacturer's information on trademarks, see page 122.

*2 For torque specifications, see page 124

*3 Alloy recommendation: Bio PontoStar® XL (BEGO, REF 61140)/Bio PontoStar® (BEGO, REF 61104)


*5 Platform Switch Design

Hybrid restoration

Ball attachment abutments					
Description	REF	Colour code	Size	Compatibility	Units
Sub-Tec ball attachment comprising: • sub ball attachment with no female part • spacer Material: Titanium alloy Tool: Insertion tool Ball attachment *2	57631		GH 0	S / RI 3.25–3.75	1
	57633		GH 3	S / RI 3.25–3.75	1
	57635		GH 5	S / RI 3.25–3.75	1
	57632		GH 0	S / RI 4.1–4.5	1
	57634		GH 3	S / RI 4.1–4.5	1
	57636		GH 5	S / RI 4.1–4.5	1
Insertion tool for ball attachment with ratchet connection	55880				1



Ball attachment impression set ² Dalbo®					
Description	REF	Colour code	Size	Compatibility	Units
Ball attachment impression set ²Dalbo®-PLUS impression on ball attachment comprising: • impression cap for ball attachment (red) • implant analog for ball attachment	55768				1



Ball attachment female parts ² Dalbo®					
Description	REF	Colour code	Size	Compatibility	Units
Female parts ²Dalbo®-PLUS comprising: • female parts ² Dalbo®-PLUS, complete (incl. retention insert) • placeholder Material: Titanium grade 4 Tool: ² Dalbo®-PLUS activator / deactivator	55769				1
²Dalbo®-PLUS activator / deactivator	55773				1
Retention insert ²Dalbo®-PLUS Material: Precious metal Tool: ² Dalbo®-PLUS activator / deactivator	55776				1



Hybrid restoration

Easy-Con abutments					
Description	REF	Colour code	Size	Compatibility	Units
Sub-Tec Easy-Con abutment Material: Titanium alloy with TiN coating Tool: Insertion tool ³ Locator® * ²	57743	■ ■	L1	S / RI 3.75–4.1	1
	57744	■ ■	L2	S / RI 3.75–4.1	1
	57745	■ ■	L3	S / RI 3.75–4.1	1
	57746	■ ■	L4	S / RI 3.75–4.1	1
	57747	■	L1	S / RI 4.5	1
	57748	■	L2	S / RI 4.5	1
	57749	■	L3	S / RI 4.5	1
	57750	■	L4	S / RI 4.5	1
Insertion tool ³Locator® with ratchet connection (also for Easy-Con)	57008				1



Easy-Con impression					
Description	REF	Colour code	Size	Compatibility	Units
Easy-Con impression coping Impression on Easy-Con	57751				4
Easy-Con analog	57760				4



Note: For manufacturer's information on trademarks, see page 122.













*² For torque specifications, see page 124

*⁵ Platform Switch Design

Hybrid restoration

Easy-Con female parts					
Description	REF	Colour code	Size	Compatibility	Units
Easy-Con laboratory set comprising: • retention insert transparent, pink and blue • block-out ring • retention cap • fabrication insert, black Material: Titanium alloy / polyamide (PA12) Tool: Easy-Con instrument	57752				2
Easy-Con instrument for screw-fitting, removing and repositioning the retention inserts, insertion aid for Easy-Con abutment	57753				1
Easy-Con fabrication insert (black) Material: Polyamide (PA12)	57754				4
Easy-Con retention insert (blue) Withdrawal force: 680 g; 6.7 N; 0–10° Material: Polyamide (PA12)	57755				4
Easy-Con retention insert (pink) Withdrawal force: 1361 g; 13.4 N; 0–10° Material: Polyamide (PA12)	57756				4
Easy-Con retention insert (transparent) Withdrawal force: 2268 g; 22.3 N; 0–10° Material: Polyamide (PA12)	57757				4
Easy-Con retention insert (red) Withdrawal force: 680 g; 6.7 N; 10–20° Material: Polyamide (PA12)	57758				4
Easy-Con retention insert (green) Withdrawal force: 1814 g; 17.8 N; 10–20° Material: Polyamide (PA12)	57759				4

Screws

Prosthesis screws						
Description	REF	Colour code	Size	Compatibility	Units	
Prosthesis screw Hex 1.25 mm	53999			Sub-Tec gold cast-on, Sub-Tec provisional abutment, Sub-Tec provisional PEEK abutment, Sub-Tec titanium abutment, Sub-Tec bar system (until Q2 2013), Sub-Tec CAD positioner, healing posts individual Ø 7	1	
Prosthesis screw for ceramic abutment	56094			BeCe® Sub-Tec ceramic abutment	1	
Prosthesis screw Sub-Tec ^{Plus}	57031			CAD SP, ST PMB, Sub-Tec ^{Plus} abutments (straight and angled), BeCe® Sub-Tec ^{Plus} ceramic abutments, Sub-Tec CAD/CAM titanium adhesive abutments, Sub-Tec provisional titanium abutments, Sub-Tec bar system (from Q2 2013), Sub-Tec CAD/CAM TiBase L	1	
Prosthesis screws Sub-Tec Universal	55534			Sub-Tec Universal	3.25–4.5	
	55535			Sub-Tec Universal	5.5	
Secondary screw Multi ^{Plus} (M1.4)	57534			Multi ^{Plus} System	1	
Prosthesis screw Multi ^{Plus} (M1.8)	57535			Sub-Tec Multi ^{Plus} 20/30°	1	

*⁵ Platform Switch Design



OVERVIEW

Large-scale models

120

Demonstration material

121

Large-scale models					
Description	REF	Colour code	Size	Compatibility	Units
Large-scale models – demonstration suitcase	57328				1
BEGO Semados® SCX implant large-scale model	58242				1
BEGO Semados® RSX implant large-scale model	56750				1
BEGO Semados® RI* ¹ implant large-scale model	58322				1
BEGO Semados® Mini implant large-scale model	57095				1
Acrylic block PS-Line (Large-scale model scale 2:1) comprising: <ul style="list-style-type: none"> • acrylic block • an SCX and RSX implant Ø4.1 L11.5 • PS TTiA (provisional abutment Platform Switch) • PS TiB (adhesive abutment Platform Switch) • PS TiAA, 15° P GH 1–2 (solid abutment titanium Platform Switch) • PS TiAA, 20° E GH 2.5–4 (solid abutment titanium Platform Switch) • prosthesis screw • Allen wrench 	56753				1



*¹ New version of the BEGO Semados® RI implants, with Platform Switch Design

Demonstration material					
Description	REF	Colour code	Size	Compatibility	Units
Maxilla demonstration model transparent acrylic model with implants	58243			SCX implants	1
	56755			RSX implants	1
BEGO Semados® SC demo implants incl. cover screw and titanium insertion posts Material: Titanium (packed non-sterile) Not for use on patients!	58244				1
BEGO Semados® SCX demo implants incl. cover screw and titanium insertion posts Material: Titanium (packed non-sterile) Not for use on patients!	58245				1
BEGO Semados® RS demo implants incl. cover screw and titanium insertion posts Material: Titanium (packed non-sterile) Not for use on patients!	56751				1
BEGO Semados® RSX demo implants incl. cover screw and titanium insertion posts Material: Titanium (packed non-sterile) Not for use on patients!	56752				1
BEGO Semados® RSX demo implants Ø3.0 incl. cover screw and titanium insertion posts Material: Titanium (packed non-sterile) Not for use on patients!	57699				1
BEGO Semados® RI*1 demo implants incl. cover screw and titanium insertion posts Material: Titanium (packed non-sterile) Not for use on patients!	58345				1
BEGO Semados® Mini demo implants incl. cover screw and titanium insertion posts Material: Titanium (packed non-sterile) Not for use on patients!	55709				1



Demonstration material					
Description	REF	Colour code	Size	Compatibility	Units
TJL (training case)	57464			Mandible	1
TJU (training case)	57465			Maxilla	1



Note:
²Dalbo® is a registered trademark of Cendres & Métaux SA, Biel/Bienne, Switzerland.
³Locator® is a registered trademark of ZEST Anchors LLC, CA, USA.
⁴DOLDER® is a registered trademark of Professor Fritz Dolder, Walisellen, Switzerland & Dr Charlotte Fleischer-Dolder, Winterthur, Switzerland.



OVERVIEW

Torque specifications	124
Material specifications	126
Index by article numbers	130
Alphabetical index	144

Torque specifications for BEGO Semados®	
Article name	Torque [Ncm]
Implant cover screw	10
Healing posts	10
Healing posts, individual	15
Impression posts	10
CAD positioner (polyetheretherketone)	10
CAD positioner (titanium grade 4)	15
CAD SP	15
Temporary restorations <ul style="list-style-type: none"> • PS ITA Ø3.0–5.5 (provisional abutment Platform Switch) • PS PPA Ø3.25–5.5 (provisional abutment Platform Switch) • PS TPA Ø3.25–5.5 (provisional abutment Platform Switch) • PS TTiA/PS TTiA NH Ø3.25–5.5 (provisional abutment Hex/no Hex Platform Switch) • Sub-Tec provisional abutment (PEEK) • Sub-Tec provisional titanium abutment 	15
Sub-System <ul style="list-style-type: none"> • BeCe® Sub-Tec ceramic abutment • BeCe® Sub-Tec^{Plus} ceramic abutment • ST PMB (CAD/CAM milling blank) • Sub-Tec CAD/CAM TiBase L • Sub-Tec CAD/CAM titanium adhesive abutment • Sub-Tec Easy-Con • Sub-Tec gold cast-on • Sub-Tec ball attachment • Sub-Tec Universal • Sub-Tec^{Plus} titanium abutment 	30
Sub-Tec Multi^{Plus} abutment	30
Multi^{Plus} System <ul style="list-style-type: none"> • Multi^{Plus} gold cast-on • Multi^{Plus} MC (Multi^{Plus} Easy-Con abutment) • Multi^{Plus} titanium abutment • Multi^{Plus} Universal 	20
Platform Switch system Ø3.0 <ul style="list-style-type: none"> • PS TiA/PS TiAA Ø3.0 (solid abutment titanium Platform Switch) • PS TiB Ø3.0 (adhesive abutment Platform Switch) 	20
Platform Switch system Ø3.25–5.5 <ul style="list-style-type: none"> • PS BA Ø3.25–4.5 (ball attachment Platform Switch) • PS CA/PS CATi Ø3.25–5.5 (ceramic abutment Platform Switch) • PS Easy-Con Ø3.75–4.5 (Easy-Con abutment Platform Switch) • PS GCO/PS GCO NH Ø3.25–5.5 (gold cast-on abutment Hex/no Hex Platform Switch) • PS Multi^{Plus} Ø3.25–4.5 (Multi^{Plus} abutment Platform Switch) • PS OCP (restoration set Platform Switch) • PS PMB (CAD/CAM milling blank Platform Switch) • PS TiA/PS TiAA Ø3.75–5.5 (solid abutment titanium Platform Switch) • PS TiB /PS TiB NH Ø3.25–5.5 (adhesive abutment Hex/no Hex Platform Switch) • PS TiBA Ø3.25–4.5 (bar abutment titanium Platform Switch) • PS UNI /PS UNI NH Ø3.25–5.5 (universal abutment Hex/no Hex Platform Switch) 	30
Mini system <ul style="list-style-type: none"> • Easy-Con Mini • Gold cast-on Mini • Ball attachment Mini • TiA (solid abutment titanium) • TiBA (bar abutment titanium) 	25

Note: For manufacturer's information on trademarks, see page 122.

General information

To avoid damage to the components, only original BEGO Implant Systems tools and products may be used for processing. The use of the torque wrench in particular is necessary to comply with the prescribed pre-tensioning of the connecting screws (specification in Ncm).

- Ensure that the prosthesis screws are not used in the laboratory or are damaged beforehand.
- After the definitive screw-fitting of the implant abutments, all connecting screws must again be tightened/checked after about 5 to 10 minutes using the prescribed torque.
- The implant/prosthesis interfaces must be regularly checked for a firm seat and to ensure that there are no gaps.
- If extremely high loads are exerted on the components, under some circumstances the screw(s) may loosen. The reason for this must be determined and eliminated.
- It is recommended that those implant abutments that are screwed into the implant with a separate prosthesis screw are screw-fixed with a new prosthesis screw after loosening the screw, e.g., to clean the prosthetic restoration / implant abutments.

All specifications have been determined on the basis of many years of practical experience to the best of our knowledge and apply to restorations that have been carried out on the basis of both our and generally valid scientific knowledge.

General information on titanium

Titanium is a biopassive or bioinert substance that is extremely taste neutral, radiotransparent and resistant to corrosion and is a poor conductor of heat (specific thermal conductivity 0.168 to gold 3.118).

In implant dentistry, pure titanium and titanium alloys are used but pure titanium does nevertheless contain impurities. Pure titanium is divided into 4 levels (grades) based on the proportion of impurities.

In all 4 groups, there are maximum amounts specified for the level of N (0.05%), C (0.08%) and H (0.015%). These substances are unavoidable because they result from the production of the titanium or are deliberately added to control the physical properties.

Pure titanium (grades 1–4) and titanium alloys (from grade 5 onwards) can be used for all dental technical work. Crowns and bridges made from titanium can be veneered with special ceramics which must be fired at temperatures of less than 800°C because of the structural transformation of the titanium at 882°C (volume transition) and have a specific coefficient of

thermal expansion (titanium: coefficient of thermal expansion of about 9.6).

When finishing and polishing the poor thermal conductivity of titanium must be noted. During processing, heat may accumulate in localised areas, leading to increased O₂ deposits, which can in turn lead to the material becoming brittle.

Because titanium becomes greasy during cutting, special mills must be used. Freshly polished surfaces retain their specular finish only if they do not come into contact with H₂O for at least 10 minutes.

During this time, a surface oxide forms that acts as a protective layer. When modelling frameworks, note that when casting titanium a thick, hard oxide layer that contains components of the embedding mass, the α-case layer, is produced. This layer must be completely removed. The edges of the model must be made thicker and are adjusted during finishing. Titanium and titanium alloys can only be joined by welding (laser, plasma, arc, resistance).

Titanium				
Elements	Grade 2	Grade 3	Grade 4	Grade 5
Nitrogen, max [%]	0.03	0.05	0.05	0.05
Carbon, max [%]	0.08	0.08	0.08	0.08
Hydrogen, max [%]	0.015	0.015	0.015	0.015
Iron, max [%]	0.3	0.3	0.5	0.4
Oxygen, max [%]	0.25	0.35	0.4	0.2
Aluminium [%]				5.5–6.75
Vanadium [%]				3.5–4.5
Titanium [%]	Remainder	Remainder	Remainder	Remainder

Note: For manufacturer's information on trademarks, see page 122.

Compositions	
Material	Article
Pure titanium grade 4 as defined by ASTM F67	BEGO Semados® S/SC/SCX/RS/R SX/RI / Mini implants
	Drill sleeves 1.6/2.5/3.2
	CADP/CADP Multi ^{Plus} (CAD positioner)
	² Dolder® bar joint attachment 3.0 – titanium
	Implant cover screws
	Female parts ³ Dolder®-PLUS, female parts
	Paralleling posts S/RS/R SX/RI/Mini-Line
	PS CADP (CAD positioner Platform Switch)
	PS TiBA (bar abutment titanium Platform Switch)
	Sub-Tec CAD positioner
	TiBA (bar abutment titanium)
Titanium grade 5 (titanium alloy Ti-6Al-4V) as defined by ASTM F136	Impression posts
	Healing posts
	Assortment set Platform Switch 0°/15°/20°
	BEGO Guide master sleeves / spoons
	BEGO Semados® Provisional Implant (PI)
	BEGO Semados® insertion posts on implants
	Bone Profiler – guide sleeve
	CAD SP (scansupport)
	Drill stops
	Easy-Con impression coping – cap, analog, retention cap
	Easy-Con Mini (with titanium nitride coating)
	Insertion tool for implants
	Mini-Line ball attachment
	Model implants S/RS/R SX/RI/Mini-Line
	Multi ^{Plus} healing caps, impressions, implant analog, protection analog, titanium abutment, MC (with titanium nitride coating)
	OCP A (implant analog)
	Open impression Mini, Mini impression posts
	PI bending instrument, PI implant analog, PI multifunctional cap, PI paralleling post
	Prosthesis screws / technician screws
	PS BA (ball attachment abutment Platform Switch)
	PS BA (ball attachment abutment Platform Switch), spacer
	PS Easy-Con (Easy-Con abutment Platform Switch) (with titanium nitride coating)
	PS HP/PS HPW (healing post Platform Switch)
	PS ITA (provisional abutment Platform Switch)
	PS Multi ^{Plus} (Multi ^{Plus} abutment Platform Switch)
	PS OCP, OCP abutment (restoration set Platform Switch)

Compositions	
Material	Article
Titanium grade 5 (titanium alloy Ti-6Al-4V) as defined by ASTM F136	PS PMB (CAD/CAM milling blank Platform Switch)
	PS TiA (solid abutments Platform Switch)
	PS TiAA (solid abutments Platform Switch)
	PS TiB / PS TiB NH (adhesive abutment Platform Switch)
	PS TTiA / PS TTiA NH (provisional abutment Platform Switch)
	PS UNI/PS UNI NH (Universal base Hex/no Hex Platform Switch), Universal base Hex/no Hex
	ST PMB (CAD/CAM milling blank)
	Sub-Tec CAD/CAM TiBase L
	Sub-Tec CAD/CAM titanium adhesive abutment Hex/no Hex
	Sub-Tec Easy-Con abutment (with titanium nitride coating)
	Sub-Tec ball attachment
	Sub-Tec ball attachment, spacer
	Sub-Tec Multi ^{Plus} abutment
	Sub-Tec immediate temporary abutment
	Sub-Tec Universal/no Hex, Universal base Hex/no Hex
	Sub-Tec ^{Plus} titanium abutment /titanium angulated abutment
	TiA (solid abutment titanium)
Stainless steel	BEGO Guide preparation instruments /instruments, bone profilers, initial drills, tissue punches, pilot drills, pilot markers, depth drills, countersinks, threadformers, screw tappers, shape drills, gap-cutter discs, trepan drills
	PI removal tool / insertion tool / stabiliser
Polyetheretherketone (PEEK)	Healing posts, individual Ø 7
	PI protection cap
	PS OCP, multifunctional cap (restoration set Platform Switch)
	PS PPA/PS TPA (provisional abutment Platform Switch)
	Sub-Tec provisional abutment Ø 7, Sub-Tec provisional PEEK abutment
Zirconium oxide	BeCe® Sub-Tec ceramic abutments / BeCe® Sub-Tec ^{Plus} ceramic abutments
	PS CA/PS CATi (ceramic abutments Platform Switch)
60Au–19Pt–20Pd–1Ir	Gold cast-on Mini, cast-on abutment Mini
	Multi ^{Plus} gold cast-on, Multi ^{Plus} cast-on abutment
	PS GCO/PS GCO NH (gold cast-on abutment Hex/no Hex Platform Switch), cast-on abutment Hex/no Hex
	Sub-Tec gold cast-on /no Hex, Sub- cast-on abutment /no Hex
69Au–12Ag–11Cu–4Pd–3Pt	Female parts ² Dalbo®-PLUS, retention insert ² Dalbo®-PLUS

Compositions	
Material	Article
Polyoxymethylene (POM)	Female parts ² Dalbo®-PLUS, placeholder
	Multi ^{Plus} Universal, wax-up sleeve gold cast-on
	PS CTI (impression set (closed) Platform Switch), impression post cap
	PS UNI/PS UNI NH (Universal abutment Hex/no Hex Platform Switch), wax-up sleeve Universal
	Sub-Dent closed tray impression, impression post cap
	Sub-Tec Universal/no Hex, sub-wax-up sleeve Universal
Polycarbonate (PC)	LCC, LCB (laboratory caps)
	PS GCO/PS GCO NH (gold cast-on abutment Hex/no Hex Platform Switch), wax-up sleeve gold cast-on
	Sub-Tec gold cast-on /no Hex, sub-wax-up sleeve gold cast-on
Polyamide (PA)	Easy-Con impression coping, fabrication insert
	Easy-Con retention insert

REF	Article	Page
53735	Internal reamer for gold cast-on abutment	79, 109
53762	Technician screw L9	89
53872	Depth gauge, S-Line	58
53888	X-ray template, S implants	16
53889	Measuring spheres	16
53897	Guiding wrench	57
53948	Hexagon screwdriver 1.25mm long, with ratchet connection	60
53949	Hexagon screwdriver 1.25mm short, with ratchet connection	60
53952	Slot screwdriver long, with ratchet connection	60
53953	Slot screwdriver short, with ratchet connection	60
53999	Prosthesis screw Hex 1.25mm	90, 118
55505	Implant cover screw, S 3.25	100
55512	Drill sleeves, for pilot drill / pilot marker Ø 1.6mm	16
55513	Drill sleeves, for depth drill Ø2.5mm	16
55523	Fibreglass pen	58
55524	Replacement brush for the fibreglass pen	58
55525	Sub-Tec Universal, S/RI 3.25–3.75	108
55526	Sub-Tec Universal no Hex, S/RI 3.25–3.75	108
55527	Sub-Tec Universal, S/RI 4.5	108
55528	Sub-Tec Universal no Hex, S/RI 4.5	108
55529	Sub-Tec Universal, S/RI 5.5	108
55530	Sub-Tec Universal no Hex, S/RI 5.5	108
55534	Prosthesis screw Sub-Tec Universal, S/RI 3.25–4.5	118
55535	Prosthesis screw Sub-Tec Universal, S/RI 5.5	118
55536	Internal reamer Universal	78, 108
55537	External reamer Universal	78, 108
55539	Sub-Dent closed tray impression, S / RI 3.75	104
55540	Sub-Dent open tray impression, S / RI 3.75	104
55551	Sub-Dent closed tray impression, S / RI 5.5	104
55563	Hexagon screwdriver 1.25mm, contra-angle short	60
55564	Hexagon screwdriver 1.25mm, contra-angle long	60
55590	Healing posts, Ø4.0 L3, S/RI 3.25–3.75	100
55591	Healing posts, Ø4.0 L5, S/RI 3.25–3.75	100
55592	Healing posts, Ø4.0 L7, S/RI 3.25–3.75	100
55593	Healing posts, Ø5.0 L3, S/RI 3.25–4.5	100
55594	Healing posts, Ø5.0 L5, S/RI 3.25–4.5	100
55595	Healing posts, Ø5.0 L7, S/RI 3.25–4.5	100
55599	BEGO Semados® ratchet adapter	35, 58, 60
55608	Implant cover screw, S / RI 3.75	100
55615	Implant cover screw, S / RI 4.1	100
55616	Implant cover screw, S / RI 4.5	100

REF	Article	Page
55617	Sub-Dent closed tray impression, S / RI 4.1	104
55618	Sub-Dent closed tray impression, S / RI 4.5	104
55619	Sub-Dent open tray impression, S / RI 4.1	104
55620	Sub-Dent open tray impression, S / RI 4.5	104
55622	Sub-Tec Universal, S/RI 4.1	108
55623	Sub-Tec Universal no Hex, S/RI 4.1	108
55624	Sub-Tec gold cast-on, S/RI 4.1	109
55625	Sub-Tec gold cast-on no Hex, S/RI 4.1	109
55709	BEGO Semados® Mini demo implant	121
55714	Initial drill, Mini-Line	55
55715	Drill stops, S/SC/SCX 4.1	48
55745	X-ray template, RI implants	16
55746	Depth gauge, RI-Line	58
55752	Pilot drill short, S-Line	46
55766	Threadformer, RI 3.25	53
55768	Ball attachment impression set Dalbo®-PLUS	85, 96, 115
55769	Female parts Dalbo®-PLUS	85, 96, 115
55773	Dalbo®-PLUS activator / deactivator	85, 96, 115
55776	Retention insert Dalbo®-PLUS	85, 96, 115
55799	Ratchet / torque wrench	58, 60
55804	Drill stops, depth drill 2.5 and S/SC/SCX 3.25–3.75	48
55810	Drill stops, S/SC/SCX 4.5	48
55811	Pilot drill long, S-Line	46
55815	Trepan drill, Ø5.0 external / Ø4.1 internal	56
55816	Trepan drill, Ø6.0 external / Ø5.1 internal	56
55817	Trepan drill, Ø4.2 external / Ø3.7 internal	56
55826	Prosthetic kit	60
55830	Insertion tool for implants long, with ratchet connection	57
55831	Insertion tool for implants short, with ratchet connection	57
55832	Insertion tool for implants long, with contra-angle connection	57
55860	Sub-Dent closed tray impression, S 3.25	104
55861	Sub-Dent open tray impression, S 3.25	104
55862	Sub-Tec gold cast-on, S/RI 3.25–3.75	109
55863	Paralleling post, S-Line	57
55873	Sub-Tec gold cast-on no Hex, S/RI 3.25–3.75	109
55880	Insertion tool for ball attachment	85, 96, 115
55908	Implant cover screw, S / RI 5.5	100
55910	Drill stops, S/SC/SCX 5.5	48
55928	DOLDER® bar joint attachment 3.0 – titanium	88, 94
55951	Sub-Tec provisional abutment Ø7, S/RI 3.25–5.5	105
55953	Healing post individual Ø7, S / RS / RSX / RI-Line	29, 100

Note: For manufacturer's information on trademarks, see page 122.

*1 New version of the BEGO Semados® RI implants, with Platform Switch Design

REF	Article	Page
56092	BeCe® Sub-Tec ceramic abutment, S/RI 3.25–5.5	106
56094	Prosthesis screw for ceramic abutment	90, 118
56300	Healing post, Ø4.5 L3, S/RI 3.25–4.5	100
56301	Healing post, Ø4.5 L5, S/RI 3.25–4.5	100
56302	Healing post, Ø4.5 L7, S/RI 3.25–4.5	100
56303	Healing post, Ø6.0 L3, S/RI 3.25–5.5	100
56304	Healing post, Ø6.0 L5, S/RI 3.25–5.5	100
56305	Healing post, Ø6.0 L7, S/RI 3.25–5.5	100
56317	Sub-Tec gold cast-on, S/RI 4.5	109
56325	Sub-Tec gold cast-on no Hex, S/RI 4.5	109
56500	Sub-Dent open tray impression, S / RI 5.5	104
56510	Sub-Tec gold cast-on, S/RI 5.5	109
56515	Sub-Tec gold cast-on no Hex, S/RI 5.5	109
56694	Model implant, S 3.25	104
56695	Model implant, S / RI 3.75	104
56696	Model implant, S / RI 4.1	104
56698	Model implant, S / RI 4.5	104
56699	Model implant, S / RI 5.5	104
56748	IDC, S/SC/SCX/RS/R SX/RI 3.25–5.5 (implant adjustment instrument)	57
56749	IDC, RS/R SX 3.0 (implant adjustment instrument)	57
56750	BEGO Semados® RSX implant large-scale model	120
56751	BEGO Semados® RS demo implant	121
56752	BEGO Semados® RSX demo implant	121
56753	Acrylic block PS-Line (large-scale model, scale 2:1)	120
56755	Maxilla demonstration model, RSX implants	121
56947	BEGO Semados® implant, Mini 2.7 L11.5	32
56948	BEGO Semados® implant, Mini 2.7 L13	32
56949	BEGO Semados® implant, Mini 2.7 L15	32
56950	BEGO Semados® implant, Mini 2.9 L11.5	32
56951	BEGO Semados® implant, Mini 2.9 L13	32
56952	BEGO Semados® implant, Mini 2.9 L15	32
56953	BEGO Semados® implant, Mini 3.1 L11.5	32
56954	BEGO Semados® implant, Mini 3.1 L13	32
56955	BEGO Semados® implant, Mini 3.1 L15	32
56956	Implant cover screw Mini	32
56957	Healing post Mini, Ø3.5 L3, Mini 2.7–3.1	32
56958	Healing post Mini, Ø3.5 L4, Mini 2.7–3.1	32
56959	Open tray impression Mini	92
56968	Ball attachment Mini, GH 1.5, Mini 2.9–3.1	96
56970	Mini-/Osseo®Plus tray	55
56972	Paralleling post, Mini-Line	57
56979	Threadformer, Mini 2.7	55
56980	Threadformer, Mini 2.9	55
56981	Threadformer, Mini 3.1	55
56982	Model implant Mini	92

REF	Article	Page
56983	Prosthesis screw Mini	97
56984	Technician screw Mini	97
56985	Gap-cutter disc (Mini-Line)	55
56986	Gap-cutter drill (Mini-Line)	55
56990	Insertion tool for implants short, with contra-angle connection	57
56991	Trepan drill, Ø5.0 external / Ø4.3 internal	56
57008	Insertion tool Locator®	86, 94, 116
57010	X-ray template, Mini implants	16
57028	Technician screw Sub-Tec®Plus	89
57031	Prosthesis screw Sub-Tec®Plus	90, 118
57055	Ball attachment Mini, GH 4, Mini 2.9–3.1	96
57056	Tissue punch, S / SC/SCX/RS/R SX/RI 3.25–3.75	46, 49, 52
57057	Tissue punch, S / SC/SCX/RS/R SX/RI 4.1	46, 49, 52
57058	Tissue punch, S / SC/SCX/RS/R SX/RI 4.5	46, 49, 52
57059	Tissue punch, S / SC/SCX/RS/R SX/RI 5.5	46, 49, 52
57060	Sub-Tec CAD positioner, S/RI 3.25–5.5	102
57095	BEGO Semados® Mini implant large-scale model	120
57100	Depth drill 2.5 short, S-Line	46
57101	Depth drill 2.5 long, S-Line	46
57102	Depth drill short, S/SC/SCX 3.25	47
57103	Depth drill long, S/SC/SCX 3.25	47
57104	Depth drill short, S/SC/SCX 3.75	47
57105	Depth drill long, S/SC/SCX 3.75	47
57106	Depth drill short, S/SC/SCX 4.1	47
57107	Depth drill long, S/SC/SCX 4.1	47
57108	Depth drill short, S/SC/SCX 4.5	47
57109	Depth drill long, S/SC/SCX 4.5	47
57110	Depth drill short, S/SC/SCX 5.5	47
57116	Sub-Tec®Plus titanium abutment GH 1–2, S/RI 3.25–3.75	106
57117	Sub-Tec®Plus titanium abutment GH 2.5–4, S/RI 3.25–3.75	106
57120	Sub-Tec®Plus titanium abutment GH 1–2, S/RI 4.1	106
57121	Sub-Tec®Plus titanium abutment GH 2.5–4, S/RI 4.1	106
57124	Sub-Tec®Plus titanium abutment GH 1–2, S/RI 4.5	106
57125	Sub-Tec®Plus titanium abutment GH 2.5–4, S/RI 4.5	106
57128	Sub-Tec®Plus titanium abutment GH 1–2, S/RI 5.5	106
57129	Sub-Tec®Plus titanium abutment GH 2.5–4, S/RI 5.5	106
57130	BEGO Guide DS (drill sleeves for guided surgery)	44
57132	Sub-Tec®Plus titanium angulated abutment, 15° P GH 1–2, S/RI 3.25–3.75	107
57133	Sub-Tec®Plus titanium angulated abutment, 15° P GH 2.5–4, S/RI 3.25–3.75	107
57134	Sub-Tec®Plus titanium angulated abutment, 15° E GH 1–2, S/RI 3.25–3.75	107

REF	Article	Page
57135	Sub-Tec ^{Plus} titanium angulated abutment, 15° E GH 2.5–4, S/RI 3.25–3.75	107
57136	Sub-Tec ^{Plus} titanium angulated abutment, 15° P GH 1–2, S/RI 4.1	107
57137	Sub-Tec ^{Plus} titanium angulated abutment, 15° P GH 2.5–4, S/RI 4.1	107
57138	Sub-Tec ^{Plus} titanium angulated abutment, 15° E GH 1–2, S/RI 4.1	107
57139	Sub-Tec ^{Plus} titanium angulated abutment, 15° E GH 2.5–4, S/RI 4.1	107
57140	Sub-Tec ^{Plus} titanium angulated abutment, 15° P GH 1–2, S/RI 4.5	107
57141	Sub-Tec ^{Plus} titanium angulated abutment, 15° P GH 2.5–4, S/RI 4.5	107
57142	Sub-Tec ^{Plus} titanium angulated abutment, 15° E GH 1–2, S/RI 4.5	107
57143	Sub-Tec ^{Plus} titanium angulated abutment, 15° E GH 2.5–4, S/RI 4.5	107
57144	Sub-Tec ^{Plus} titanium angulated abutment, 15° P GH 1–2, S/RI 5.5	107
57145	Sub-Tec ^{Plus} titanium angulated abutment, 15° P GH 2.5–4, S/RI 5.5	107
57146	Sub-Tec ^{Plus} titanium angulated abutment, 15° E GH 1–2, S/RI 5.5	107
57147	Sub-Tec ^{Plus} titanium angulated abutment, 15° E GH 2.5–4, S/RI 5.5	107
57212	BEGO OSS, particle size 0.5–1 mm, 0.5 mL	10
57213	BEGO OSS, particle size 0.5–1 mm, 1 mL	10
57214	BEGO OSS, particle size 0.5–1 mm, 3 mL	10
57215	BEGO OSS, particle size 1–2 mm, 2 mL	10
57216	BEGO OSS, particle size 1–2 mm, 5 mL	10
57217	BEGO OSS S, particle size 0.5–1 mm, 0.5 mL	10
57218	BEGO OSS S, particle size 0.5–1 mm, 1 mL	10
57219	BEGO OSS S, particle size 0.8–1.5 mm, 2 mL	10
57220	BEGO Collagen Fleece	10
57221	BEGO Collagen Membrane, 15 × 20 mm	10
57222	BEGO Collagen Membrane, 20 × 30 mm	10
57223	BEGO Collagen Membrane, 30 × 40 mm	10
57252	Healing post Mini, Ø3.5 L7, Mini 2.7–3.1	32
57265	Drill extension one-part (without internal cooling)	57
57266	Hexagon screwdriver 1.25 mm XS, with ratchet connection	60
57285	Sub-Tec CAD/CAM titanium adhesive abutment, S/RI 3.25–3.75	102
57286	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 3.25–3.75	102

REF	Article	Page
57287	Sub-Tec CAD/CAM titanium adhesive abutment, S/RI 4.1	102
57288	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 4.1	102
57289	Sub-Tec CAD/CAM titanium adhesive abutment, S/RI 4.5	102
57290	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 4.5	102
57291	Sub-Tec CAD/CAM titanium adhesive abutment, S/RI 5.5	102
57292	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 5.5	102
57300	Sub-Tec provisional titanium abutment no Hex, S/RI 3.25–3.75	105
57301	Sub-Tec provisional titanium abutment no Hex, S/RI 4.1	105
57302	Sub-Tec provisional titanium abutment no Hex, S/RI 4.5	105
57303	Sub-Tec provisional titanium abutment no Hex, S/RI 5.5	105
57304	Sub-Tec provisional titanium abutment, S/RI 3.25–3.75	105
57305	Sub-Tec provisional titanium abutment, S/RI 4.1	105
57306	Sub-Tec provisional titanium abutment, S/RI 4.5	105
57307	Sub-Tec provisional titanium abutment, S/RI 5.5	105
57308	Depth drill short, S-Line	46
57309	Depth drill long, S-Line	46
57320	Gold cast-on Mini, Mini 2.9–3.1	93
57321	Prosthesis screw Mini, conical	97
57322	Technician screw Mini, conical	97
57323	Internal reamer for gold cast-on Mini	93
57324	Healing post conical, S/RI 3.25–3.75	100
57328	Large-scale models – demonstration suitcase	120
57332	Screw tapper, S/SC/SCX 3.25	47
57333	Screw tapper, S/SC/SCX 3.75	47
57334	Screw tapper, S/SC/SCX 4.1	47
57335	Screw tapper, S/SC/SCX 4.5	47
57336	Screw tapper, S/SC/SCX 5.5	47
57339	Healing post conical, S/RI 4.1	100
57340	BEGO Semados® S-Line tray ^{Plus}	46
57345	Drill stop tray ^{Plus} , S-Line	48
57347	Drill module, S/SC/SCX 5.5	46
57350	Countersink, S/SC/SCX 3.25	47
57351	Countersink, S/SC/SCX 3.75	47
57352	Countersink, S/SC/SCX 4.1	47
57353	Countersink, S/SC/SCX 4.5	47
57354	Countersink, S/SC/SCX 5.5	47
57395	BEGO Guide master sleeves, Ø4.2 (A), S/RS/RSX-Line	38, 41

Note: For manufacturer's information on trademarks, see page 122.

*1 New version of the BEGO Semados® RI implants, with Platform Switch Design

REF	Article	Page
57397	BEGO Guide master sleeves, Ø4.7 (A), S/RS/RXS-Line	38, 41
57399	BEGO Guide S-Line tray	38
57400	BEGO Guide – pilot drill short	44
57401	BEGO Guide – pilot drill long	44
57411	BEGO Guide spoon, Ø1.6 (A1), S-Line	38
57412	BEGO Guide spoon, Ø2.5 (A2), S-Line	38
57413	BEGO Guide spoon, Ø2.8 (A3), S/RS/RXS 3.25	38
57414	BEGO Guide spoon, Ø3.25 (A4), S/RS/RXS 3.75	38
57415	BEGO Guide spoon, Ø1.6 (B1), S-Line	38
57416	BEGO Guide spoon, Ø2.5 (B2), S-Line	38
57417	BEGO Guide spoon, Ø2.8 (B3), S/RS/RXS 3.25	38
57418	BEGO Guide spoon, Ø3.25 (B4), S/RS/RXS 3.75	38
57419	BEGO Guide spoon, Ø3.65 (B5), S/RS/RXS 4.1	38
57420	BEGO Guide spoon, Ø4.0 (B6), S/RS/RXS 4.5	38
57421	BEGO Guide tissue punch, Ø4.2 (A), S/ SC / SCX /RS/RXS 3.0–3.75	38, 41
57422	BEGO Guide tissue punch, Ø4.7 (B), S/ SC / SCX /RS/RXS 4.1–4.5	38, 41
57423	BEGO Guide pilot drill, Ø1.6 L18 (X1), S-Line	39
57424	BEGO Guide pilot drill, Ø1.6 L23 (Y1), S-Line	39
57425	BEGO Guide pilot drill, Ø1.6 L29 (Z1), S-Line	39
57426	BEGO Guide depth drill, Ø2.5 L18 (X2), S-Line	39
57427	BEGO Guide depth drill, Ø2.5 L23.5 (Y2), S-Line	39
57428	BEGO Guide depth drill, Ø2.5 L29 (Z2), S-Line	39
57429	BEGO Guide depth drill, Ø2.8 L18 (X3), S/RS/RXS 3.25	39
57430	BEGO Guide depth drill, Ø2.8 L23.5 (Y3), S/RS/RXS 3.25	39
57431	BEGO Guide depth drill, Ø2.8 L29 (Z3), S/RS/RXS 3.25	39
57432	BEGO Guide depth drill, Ø3.25 L18 (X4), S/RS/RXS 3.75	39
57433	BEGO Guide depth drill, Ø3.25 L23.5 (Y4), S/RS/RXS 3.75	39
57434	BEGO Guide depth drill, Ø3.25 L29 (Z4), S/RS/RXS 3.75	39

REF	Article	Page
57435	BEGO Guide depth drill, Ø3.65 L18 (X5), S/RS/RXS 4.1	39
57436	BEGO Guide depth drill, Ø3.65 L23.5 (Y5), S/RS/RXS 4.1	39
57437	BEGO Guide depth drill, Ø3.65 L29 (Z5), S/RS/RXS 4.1	39
57438	BEGO Guide depth drill, Ø4.0 L18 (X6), S/RS/RXS 4.5	39
57439	BEGO Guide depth drill, Ø4.0 L23.5 (Y6), S/RS/RXS 4.5	39
57441	BEGO Guide depth drill, Ø4.0 L29 (Z6), S/RS/RXS 4.5	39
57442	BEGO Guide countersink, (3), S/RS/RXS 3.25	39
57443	BEGO Guide countersink, (4), S/RS/RXS 3.75	39
57444	BEGO Guide countersink, (5), S/RS/RXS 4.1	39
57445	BEGO Guide countersink, (6), S/RS/RXS 4.5	39
57446	BEGO Guide screw tapper, (3), S/RS/RXS 3.25	40
57447	BEGO Guide screw tapper, (4), S/RS/RXS 3.75	40
57448	BEGO Guide screw tapper, (5), S/RS/RXS 4.1	40
57449	BEGO Guide screw tapper, (6), S/RS/RXS 4.5	40
57450	BEGO Guide connector, Ø4.2 (AX), S-Line	40
57451	BEGO Guide connector, Ø4.2 (AY), S-Line	40
57452	BEGO Guide connector, Ø4.2 (AZ), S-Line	40
57453	BEGO Guide connector, Ø4.7 (BX), S-Line	40
57454	BEGO Guide connector, Ø4.7 (BY), S-Line	40
57455	BEGO Guide connector, Ø4.7 (BZ), S-Line	40
57456	BEGO Guide depth stop ring connector, Ø4.2 (A), S/RS/RXS-Line	40, 43
57457	BEGO Guide depth stop ring connector, Ø4.7 (B), S/RS/RXS-Line	40, 43
57458	BEGO Guide ratchet adapter for connector, S-Line	40
57459	BEGO Guide centre drill, Ø4.2 (A), S/ SC / SCX /RS/RXS 3.0–3.75	39, 42
57463	BEGO Guide centre drill, Ø4.7 (B), S/ SC / SCX /RS/RXS 4.1–4.5	39, 42
57464	TJL (training case, mandible)	122
57465	TJU (training case, maxilla)	122
57467	Bone profiler, S/RI 3.25–3.75	56
57468	Bone profiler, S/RI 4.1	56
57469	Bone profiler, S/RI 4.5	56
57470	Bone profiler, S/RI 5.5	56
57476	Drill stops depth drill 2.5, RS / RSX-Line	51

REF	Article	Page
57477	Drill stops, RS/RXS 3.0	51
57478	Drill stops, RS/RXS 3.75	51
57479	Drill stops, RS/RXS 4.1–4.5	51
57480	Drill stops, RS/RXS 5.5	51
57481	Pilot marker short, RS / RSX-Line	49
57482	Pilot marker long, RS / RSX-Line	49
57483	Drill stop tray ^{Plus} , RS / RSX-Line	51
57484	DD D1, RS/RXS 3.0 (depth drill)	50
57485	DD D1, RS/RXS 3.75 (depth drill)	50
57486	DD D1, RS/RXS 4.1 (depth drill)	50
57487	DD D1, RS/RXS 4.5 (depth drill)	50
57488	DD D1, RS/RXS 5.5 (depth drill)	50
57494	Sub-Tec provisional PEEK abutment, S/RI 3.25–3.75	105
57495	Sub-Tec provisional PEEK abutment, S/RI 4.1–4.5	105
57505	Sub-Tec Multi ^{Plus} abutments 0°, GH 1, S/RI 3.25–3.75	110
57506	Sub-Tec Multi ^{Plus} abutments 0°, GH 1, S/RI 4.1	110
57507	Sub-Tec Multi ^{Plus} abutments 0°, GH 1, S/RI 4.5	110
57508	Sub-Tec Multi ^{Plus} abutments 0°, GH 3, S/RI 3.25–3.75	110
57509	Sub-Tec Multi ^{Plus} abutments 0°, GH 3, S/RI 4.1	110
57510	Sub-Tec Multi ^{Plus} abutments 0°, GH 3, S/RI 4.5	110
57511	Sub-Tec Multi ^{Plus} abutments 20°, GH 2.3–0.6, S/RI 3.25–3.75	111
57512	Sub-Tec Multi ^{Plus} abutments 20°, GH 2.3–0.6, S/RI 4.1	111
57513	Sub-Tec Multi ^{Plus} abutments 20°, GH 2.3–0.6, S/RI 4.5	111
57514	Sub-Tec Multi ^{Plus} abutments 20°, GH 4.0–2.3, S/RI 3.25–3.75	111
57515	Sub-Tec Multi ^{Plus} abutments 20°, GH 4.0–2.3, S/RI 4.1	111
57516	Sub-Tec Multi ^{Plus} abutments 20°, GH 4.0–2.3, S/RI 4.5	111
57517	Sub-Tec Multi ^{Plus} abutments 30°, GH 4.0–1.5, S/RI 3.25–3.75	111
57518	Sub-Tec Multi ^{Plus} abutments 30°, GH 4.0–1.5, S/RI 4.1	111
57519	Sub-Tec Multi ^{Plus} abutments 30°, GH 4.0–1.5, S/RI 4.5	111
57520	Multi ^{Plus} healing cap	81, 111
57521	Multi ^{Plus} healing cap Mushroom	81, 111
57522	Multi ^{Plus} closed tray impression short	82, 112
57523	Multi ^{Plus} open tray impression	82, 112
57524	Multi ^{Plus} implant analog, 1 unit	82, 112

REF	Article	Page
57525	Multi ^{Plus} implant analogs, 4 units	82, 112
57526	Multi ^{Plus} titanium abutment	83, 113
57527	Multi ^{Plus} gold cast-on	84, 114
57530	Multi ^{Plus} adjustment supporter, 20°	80, 110
57531	Multi ^{Plus} adjustment supporter, 30°	80, 110
57532	Multi ^{Plus} insertion splint	80, 110
57533	Insertion instrument Multi ^{Plus} abutment 0°	80, 110
57534	Secondary screw Multi ^{Plus} (M1.4)	90, 118
57535	Prosthesis screw Multi ^{Plus} (M1.8)	90, 118
57536	Technician screw Multi ^{Plus} (M1.4)	89
57537	Multi ^{Plus} protection analog	83, 113
57538	Multi ^{Plus} Universal	84, 114
57539	Multi ^{Plus} external reamer	84, 114
57540	Multi ^{Plus} internal reamer	84, 114
57541	Multi ^{Plus} bone shaper, S/SC/SCX 3.75	80, 110
57542	Multi ^{Plus} bone shaper, S/SC/SCX 4.1	80, 110
57543	Multi ^{Plus} bone shaper, S/SC/SCX 4.5	80, 110
57551	Multi ^{Plus} bone shaper, S/SC/SCX 3.25	80, 110
57554	Multi ^{Plus} closed tray impression long	82, 112
57581	Pilot marker short, RI-Line	52
57582	Pilot marker long, RI-Line	52
57583	Depth drill 3.2 short, RI-Line	52
57584	Depth drill 3.2 long, RI-Line	52
57585	Depth drill short, RI 3.75	53
57586	Depth drill long, RI 3.75	53
57587	Depth drill short, RI 4.1	53
57588	Depth drill long, RI 4.1	53
57589	Depth drill short, RI 4.5	53
57590	Depth drill long, RI 4.5	53
57591	Depth drill short, RI 5.5	53
57592	Countersink, RI 3.75	53
57593	Countersink, RI 4.1	53
57594	Countersink, RI 4.5	53
57595	Countersink, RI 5.5	53
57596	Drill sleeves, for pilot drill / pilot marker Ø2.5 mm	16
57597	Drill sleeves, for depth drill Ø3.2	16
57598	Paralleling post, RI-Line	57
57607	Drill stops, depth drill 3.2, RI-Line	54
57608	Drill stops, RI 3.75–4.1	54
57609	Drill stops, RI 4.5–5.5	54
57610	Drill stop tray ^{Plus} , RI-Line	54
57612	BEGO Semados® RI-Line tray ^{Plus}	52
57613	Drill module, RI 5.5	52
57615	Threadformer, RI 3.75	53
57616	Threadformer, RI 4.1	53
57617	Threadformer, RI 4.5	53

Note: For manufacturer's information on trademarks, see page 122.

*1 New version of the BEGO Semados® RI implants, with Platform Switch Design

REF	Article	Page
57618	Threadformer, RI 5.5	53
57619	Screw tapper, RI 3.75	53
57620	Screw tapper, RI 4.1	53
57621	Screw tapper, RI 4.5	53
57622	Screw tapper, RI 5.5	53
57623	Easy-Con Mini, L1.5, Mini 3.1	94
57624	Easy-Con Mini, L2.5, Mini 3.1	94
57625	Easy-Con Mini, L3.5, Mini 3.1	94
57631	Sub-Tec ball attachment, GH0, S/RI 3.25–3.75	115
57632	Sub-Tec ball attachment, GH0, S/RI 4.1–4.5	115
57633	Sub-Tec ball attachment, GH3, S/RI 3.25–3.75	115
57634	Sub-Tec ball attachment, GH3, S/RI 4.1–4.5	115
57635	Sub-Tec ball attachment, GH5, S/RI 3.25–3.75	115
57636	Sub-Tec ball attachment, GH5, S/RI 4.1–4.5	115
57656	Sub-Tec CAD/CAM TiBase L, S/RI 3.25–3.75	103
57657	Sub-Tec CAD/CAM TiBase L, S/RI 4.1	103
57658	Sub-Tec CAD/CAM TiBase L, S/RI 4.5	103
57659	Sub-Tec CAD/CAM TiBase L, S/RI 5.5	103
57660	BEGO Semados® provisional implant (PI), 1 unit	34
57661	PI multifunctional cap, 1 unit	34
57662	PI protection cap	34
57663	PI paralleling post	35
57664	PI depth drill	35
57665	PI removal tool	35
57666	PI removal tool	35
57667	PI bending instrument	35
57668	PI ratchet	35
57669	PI stabiliser	35
57670	BEGO Semados® PI tray	34
57671	PI implant analog	34
57672	X-ray template, PI implants	16
57673	BEGO Semados® provisional implant (PI), 10 unit	34
57674	PI multifunctional cap, 5 unit	34
57680	BeCe® Sub-Tec ^{Plus} ceramic abutments, S/RI 3.25–3.75	106
57681	BeCe® Sub-Tec ^{Plus} ceramic abutments, S/RI 4.1	106
57682	BeCe® Sub-Tec ^{Plus} ceramic abutments, S/RI 4.5	106
57683	BeCe® Sub-Tec ^{Plus} ceramic abutments, S/RI 5.5	106
57686	BEGO Guide Sp, Ø2.0 (A1), RS/RXS-Line (reduction sleeve for guided surgery)	41
57687	BEGO Guide Sp, Ø2.5 (A2), RS/RXS-Line (reduction sleeve for guided surgery)	41
57688	BEGO Guide Sp, Ø2.8 (A3), RS/RXS 3.0 (reduction sleeve for guided surgery)	41

REF	Article	Page
57689	BEGO Guide Sp, Ø3.4 (A4), RS/RXS 3.75 (reduction sleeve for guided surgery)	41
57690	BEGO Guide Sp, Ø2.0 (B1), RS/RXS-Line (reduction sleeve for guided surgery)	41
57691	BEGO Guide Sp, Ø2.5 (B2), RS/RXS-Line (reduction sleeve for guided surgery)	41
57692	BEGO Guide Sp, Ø2.8 (B3), RS/RXS 3.0 (reduction sleeve for guided surgery)	41
57693	BEGO Guide Sp, Ø3.4 (B4), RS/RXS 3.75 (reduction sleeve for guided surgery)	41
57694	BEGO Guide Sp, Ø3.8 (B5), RS/RXS 4.1 (reduction sleeve for guided surgery)	41
57695	BEGO Guide Sp, Ø4.1 (B6), RS/RXS 4.5 (reduction sleeve for guided surgery)	41
57696	BEGO Guide PD, Ø2.0 L18 (X1), RS/RXS-Line (pilot drill for guided surgery)	42
57697	BEGO Guide PD, Ø2.0 L23.5 (Y1), RS/RXS-Line (pilot drill for guided surgery)	42
57698	BEGO Guide PD, Ø2.0 L29 (Z1), RS/RXS-Line (pilot drill for guided surgery)	42
57699	BEGO Semados® RSX demo implant Ø 3.0	121
57708	BEGO Semados® implant, RI 3.75 L8.5	26
57709	BEGO Semados® implant, RI 3.75 L10	26
57710	BEGO Semados® implant, RI 3.75 L11.5	26
57711	BEGO Semados® implant, RI 3.75 L13	26
57712	BEGO Semados® implant, RI 3.75 L15	26
57713	BEGO Guide DD, Ø2.5 L18 (X2), RS/RXS-Line (depth drill for guided surgery)	42
57714	BEGO Guide DD, Ø2.5 L23.5 (Y2), RS/RXS-Line (depth drill for guided surgery)	42
57715	BEGO Guide DD, Ø2.5 L29 (Z2), RS/RXS-Line (depth drill for guided surgery)	42
57716	BEGO Guide DD, Ø2.8 L18 (X3), RS/RXS 3.0 (depth drill for guided surgery)	42
57717	BEGO Guide DD, Ø2.8 L23.5 (Y3), RS/RXS 3.0	42
57718	BEGO Semados® implant, RI 4.1 L8.5	26
57719	BEGO Semados® implant, RI 4.1 L10	26
57720	BEGO Semados® implant, RI 4.1 L11.5	26
57721	BEGO Semados® implant, RI 4.1 L13	26
57722	BEGO Semados® implant, RI 4.1 L15	26
57723	BEGO Guide DD, Ø2.8 L29 (Z3), RS/RXS 3.0 (depth drill for guided surgery)	42

REF	Article	Page
57724	BEGO Guide DD, Ø3.4 L18 (X4), RS/RSX 3.75 (depth drill for guided surgery)	42
57725	BEGO Guide DD, Ø3.4 L23.5 (Y4), RS/RSX 3.75 (depth drill for guided surgery)	42
57726	BEGO Guide DD, Ø3.4 L29 (Z4), RS/RSX 3.75 (depth drill for guided surgery)	42
57727	BEGO Guide DD, Ø3.8 L18 (X5), RS/RSX 4.1 (depth drill for guided surgery)	42
57728	BEGO Semados® implant, RI 4.5 L8.5	26
57729	BEGO Semados® implant, RI 4.5 L10	26
57730	BEGO Semados® implant, RI 4.5 L11.5	26
57731	BEGO Semados® implant, RI 4.5 L13	26
57732	BEGO Semados® implant, RI 4.5 L15	26
57733	BEGO Guide DD, Ø3.8 L23.5 (Y5), RS/RSX 4.1 (depth drill for guided surgery)	42
57734	BEGO Guide DD, Ø3.8 L29 (Z5), RS/RSX 4.1 (depth drill for guided surgery)	42
57735	BEGO Guide DD, Ø4.1 L18 (X6), RS/RSX 4.5 (depth drill for guided surgery)	42
57736	BEGO Guide DD, Ø4.1 L23.5 (Y6), RS/RSX 4.5 (depth drill for guided surgery)	42
57737	BEGO Guide DD, Ø4.1 L29 (Z6), RS/RSX 4.5 (depth drill for guided surgery)	42
57738	BEGO Semados® implant, RI 5.5 L8.5	26
57739	BEGO Semados® implant, RI 5.5 L10	26
57740	BEGO Semados® implant, RI 5.5 L11.5	26
57741	BEGO Semados® implant, RI 5.5 L13	26
57743	Sub-Tec Easy-Con abutment, L1, S/RI 3.75–4.1	116
57744	Sub-Tec Easy-Con abutment, L2, S/RI 3.75–4.1	116
57745	Sub-Tec Easy-Con abutment, L3, S/RI 3.75–4.1	116
57746	Sub-Tec Easy-Con abutment, L4, S/RI 3.75–4.1	116
57747	Sub-Tec Easy-Con abutment, L1, S/RI 4.5	116
57748	Sub-Tec Easy-Con abutment, L2, S/RI 4.5	116
57749	Sub-Tec Easy-Con abutment, L3, S/RI 4.5	116
57750	Sub-Tec Easy-Con abutment, L4, S/RI 4.5	116
57751	Easy-Con impression coping	86, 94, 116
57752	Easy-Con laboratory set	87, 95, 117
57753	Easy-Con instrument	87, 95, 117
57754	Easy-Con fabrication insert (black)	87, 95, 117
57755	Easy-Con retention insert (blue)	87, 95, 117
57756	Easy-Con retention insert (pink)	87, 95, 117
57757	Easy-Con retention insert (transparent)	87, 95, 117
57758	Easy-Con retention insert (red)	87, 95, 117
57759	Easy-Con retention insert (green)	87, 95, 117
57760	Easy-Con analog	86, 94, 116

REF	Article	Page
57764	PS HP, Ø3.0 L3, RS/RSX 3.0 (healing post Platform Switch)	28
57765	PS HP, Ø3.0 L5, RS/RSX 3.0 (healing post Platform Switch)	28
57766	PS HP, Ø3.0 L7, RS/RSX 3.0 (healing post Platform Switch)	28
57767	PS HP, Ø4.0 L3, RS/RSX 3.0 (healing post Platform Switch)	28
57768	PS HP, Ø4.0 L5, RS/RSX 3.0 (healing post Platform Switch)	28
57769	PS HP, Ø4.0 L7, RS/RSX 3.0 (healing post Platform Switch)	28
57773	PS CTI, RS/RSX 3.0 (impression set (closed) Platform Switch)	72
57774	PS CTI, RS/RSX 3.0 (impression set (open) Platform Switch)	72
57776	PS TiA, GH 2.5–4, RS / RSX 3.0 (solid abutment titanium Platform Switch)	73
57778	PS ITA RS / RSX 3.0 (provisional abutment Platform Switch)	73
57781	PS TiB, RS / RSX 3.0 (adhesive abutment Platform Switch)	68
57782	PScrew (prosthesis screw)	90
57783	TScrew (technician screw)	89
57784	PScrew (prosthesis screw, for CAD positioner Platform Switch)	90
57796	PS IMPA, RS / RSX 3.0 (implant analog Platform Switch)	72
57797	PS TiAA, 15° P GH 2.5–4, RS / RSX 3.0 (solid abutment titanium Platform Switch)	73
57798	PS TiAA, 15° E GH 2.5–4, RS / RSX 3.0 (solid abutment titanium Platform Switch)	73
57799	PS CTI, SC / SCX / RS/RSX/ RI*1 3.75 (impression set (closed) Platform Switch)	72
57800	PS CTI, SC / SCX / RS/RSX/ RI*1 4.1 (impression set (closed) Platform Switch)	72
57801	PS CTI, SC / SCX / RS/RSX/ RI*1 4.5 (impression set (closed) Platform Switch)	72
57802	PS CTI, SC / SCX / RS/RSX/ RI*1 5.5 (impression set (closed) Platform Switch)	72
57803	PS CTI, SC / SCX / RS/RSX/ RI*1 3.75 (impression set (open) Platform Switch)	72
57804	PS CTI, SC / SCX / RS/RSX/ RI*1 4.1 (impression set (open) Platform Switch)	72
57805	PS CTI, SC / SCX / RS/RSX/ RI*1 4.5 (impression set (open) Platform Switch)	72

Note: For manufacturer's information on trademarks, see page 122.

*1 New version of the BEGO Semados® RI implants, with Platform Switch Design

REF	Article	Page	REF	Article	Page
57806	PS CTI, SC / SCX / RS/R SX / RI*1 5.5 (impression set (open) Platform Switch)	72	57825	PS TiB, SC/SCX/RS/R SX/RI*1 4.5 (adhesive abutment Platform Switch)	69
57807	PS HP, Ø4.5 L3, SC / SCX / RS/R SX / RI*1 3.25–3.75 (healing post Platform Switch)	28	57826	PS TiB, SC/SCX/RS/R SX/RI*1 5.5 (adhesive abutment Platform Switch)	69
57808	PS HP, Ø4.5 L5, SC / SCX / RS/R SX / RI*1 3.25–3.75 (healing post Platform Switch)	28	57827	PS TiB NH, SC/SCX/RS/R SX/RI*1 3.25–3.75 (adhesive abutment no Hex Platform Switch)	70
57809	PS HP, Ø5.0 L3, SC / SCX / RS/R SX / RI*1 4.1 (healing post Platform Switch)	28	57828	PS TiB NH, SC/SCX/RS/R SX/RI*1 4.1 (adhesive abutment no Hex Platform Switch)	70
57810	PS HP, Ø5.0 L5, SC / SCX / RS/R SX / RI*1 4.1 (healing post Platform Switch)	28	57829	PS TiB NH, SC/SCX/RS/R SX/RI*1 4.5 (adhesive abutment no Hex Platform Switch)	70
57811	PS HP, Ø5.5 L3, SC / SCX / RS/R SX / RI*1 4.5 (healing post Platform Switch)	28	57830	PS TiB NH, SC / SCX / RS/R SX / RI*1 5.5 (adhesive abutment no Hex Platform Switch)	70
57812	PS HP, Ø5.5 L5, SC / SCX / RS/R SX / RI*1 4.5 (healing post Platform Switch)	28	57831	PS UNI, SC / SCX / RS/R SX / RI*1 3.25–3.75 (universal abutment Platform Switch)	78
57813	PS HP, Ø6.5 L3, SC / SCX / RS/R SX / RI*1 5.5 (healing post Platform Switch)	28	57832	PS UNI, SC / SCX / RS/R SX / RI*1 4.1 (universal abutment Platform Switch)	78
57814	PS HP, Ø6.5 L5, SC / SCX / RS/R SX / RI*1 5.5 (healing post Platform Switch)	28	57833	PS UNI, SC / SCX / RS/R SX / RI*1 4.5 (universal abutment Platform Switch)	78
57815	PS HPW, Ø5.5 L3, SC / SCX / RS/R SX / RI*1 3.25–3.75 (healing post Platform Switch)	29	57834	PS UNI, SC / SCX / RS/R SX / RI*1 5.5 (universal abutment Platform Switch)	78
57816	PS HPW, Ø6.0 L3, SC / SCX / RS/R SX / RI*1 4.1 (healing post Platform Switch)	29	57835	PS UNI NH, SC / SCX / RS/R SX / RI*1 3.25–3.75 (universal abutment no Hex Platform Switch)	78
57817	PS HPW, Ø6.5 L3, SC / SCX / RS/R SX / RI*1 4.5 (healing post Platform Switch)	29	57836	PS UNI NH, SC / SCX / RS/R SX / RI*1 4.1 (universal abutment no Hex Platform Switch)	78
57818	PS HPW, Ø7.0 L3, SC / SCX / RS/R SX / RI*1 5.5 (healing post Platform Switch)	29	57837	PS UNI NH, SC / SCX / RS/R SX / RI*1 4.5 (universal abutment no Hex Platform Switch)	78
57819	PS IMPA, SC / SCX / RS/R SX / RI*1 3.75 (implant analog Platform Switch)	72	57838	PS UNI NH, SC / SCX / RS/R SX / RI*1 5.5 (universal abutment no Hex Platform Switch)	78
57820	PS IMPA, SC/SCX/RS/R SX/RI*1 4.1 (implant analog Platform Switch)	72	57846	PS TiA, GH 1–2, SC / SCX / RS / RSX / RI*1 3.25–3.75 (solid abutment titanium Platform Switch)	76
57821	PS IMPA, SC/SCX/RS/R SX/RI*1 4.5 (implant analog Platform Switch)	72	57847	PS TiA, GH 2.5–4, SC / SCX / RS / RSX / RI*1 3.25–3.75 (solid abutment titanium Platform Switch)	76
57822	PS IMPA, SC/SCX/RS/R SX/RI*1 5.5 (implant analog Platform Switch)	72	57848	PS TiA, GH 1–2, SC / SCX / RS / RSX / RI*1 4.1 (solid abutment titanium Platform Switch)	76
57823	PS TiB, SC/SCX/RS/R SX/RI*1 3.25–3.75 (adhesive abutment Platform Switch)	69	57849	PS TiA, GH 2.5–4, SC / SCX / RS / RSX / RI*1 4.1 (solid abutment titanium Platform Switch)	76
57824	PS TiB, SC/SCX/RS/R SX/RI*1 4.1 (adhesive abutment Platform Switch)	69	57850	PS TiA, GH 1–2, SC / SCX / RS / RSX / RI*1 4.5 (solid abutment titanium Platform Switch)	76
			57851	PS TiA, GH 2.5–4, SC / SCX / RS / RSX / RI*1 4.5 (solid abutment titanium Platform Switch)	76
			57852	PS TiA, GH 1–2, SC / SCX / RS / RSX / RI*1 5.5 (solid abutment titanium Platform Switch)	76
			57853	PS TiA, GH 2.5–4, SC / SCX / RS / RSX / RI*1 5.5 (solid abutment titanium Platform Switch)	76

REF	Article	Page
57854	PS TTiA, SC / SCX / RS/R SX / RI*1 3.25–3.75 (provisional abutment Platform Switch)	74
57855	PS TTiA, SC / SCX / RS/R SX / RI*1 4.1 (provisional abutment Platform Switch)	74
57856	PS TTiA, SC / SCX / RS/R SX / RI*1 4.5 (provisional abutment Platform Switch)	74
57857	PS TTiA, SC / SCX / RS/R SX / RI*1 5.5 (provisional abutment Platform Switch)	74
57858	PS TTiA NH, SC / SCX / RS/R SX / RI*1 3.25–3.75 (provisional abutment no Hex Platform Switch)	74
57859	PS TTiA NH, SC / SCX / RS/R SX / RI*1 4.1 (provisional abutment no Hex Platform Switch)	74
57860	PS TTiA NH, SC / SCX / RS/R SX / RI*1 4.5 (provisional abutment no Hex Platform Switch)	74
57861	PS TTiA NH, SC / SCX / RS/R SX / RI*1 5.5 (provisional abutment no Hex Platform Switch)	74
57862	BEGO Semados® implant, RSX 3.0 L10	23
57863	BEGO Semados® implant, RSX 3.0 L11.5	23
57864	BEGO Semados® implant, RSX 3.0 L13	23
57865	BEGO Semados® implant, RSX 3.0 L15	23
57866	BEGO Semados® implant, RSX 3.75 L8.5	23
57867	BEGO Semados® implant, RSX 3.75 L10	23
57868	BEGO Semados® implant, RSX 3.75 L11.5	23
57869	BEGO Semados® implant, RSX 3.75 L13	23
57870	BEGO Semados® implant, RSX 3.75 L15	23
57871	BEGO Semados® implant, RSX 4.1 L7	23
57872	BEGO Semados® implant, RSX 4.1 L8.5	23
57873	BEGO Semados® implant, RSX 4.1 L10	23
57874	BEGO Semados® implant, RSX 4.1 L11.5	23
57875	BEGO Semados® implant, RSX 4.1 L13	23
57876	BEGO Semados® implant, RSX 4.1 L15	23
57877	BEGO Semados® implant, RSX 4.5 L7	23
57878	BEGO Semados® implant, RSX 4.5 L8.5	23
57879	BEGO Semados® implant, RSX 4.5 L10	23
57880	BEGO Semados® implant, RSX 4.5 L11.5	23
57881	BEGO Semados® implant, RSX 4.5 L13	23
57882	BEGO Semados® implant, RSX 4.5 L15	23
57883	BEGO Semados® implant, RSX 5.5 L7	23
57884	BEGO Semados® implant, RSX 5.5 L8.5	23
57885	BEGO Semados® implant, RSX 5.5 L10	23
57886	BEGO Semados® implant, RSX 5.5 L11.5	23
57887	BEGO Semados® implant, RSX 5.5 L13	23
57889	PS TiA, 15° P GH 1–2, SC / SCX / RS / RSX / RI*1 3.25–3.75 (solid abutment titanium Platform Switch)	76

REF	Article	Page
57890	PS TiAA, 15° P GH 2.5–4, SC / SCX / RS / RSX / RI*1 3.25–3.75 (solid abutment titanium Platform Switch)	76
57891	PS TiAA, 15° E GH 1–2, SC / SCX / RS / RSX / RI*1 3.25–3.75 (solid abutment titanium Platform Switch)	76
57892	PS TiAA, 15° E GH 2.5–4, SC / SCX / RS / RSX / RI*1 3.25–3.75 (solid abutment titanium Platform Switch)	76
57893	PS TiAA, 15° P GH 1–2, SC / SCX / RS / RSX / RI*1 4.1 (solid abutment titanium Platform Switch)	76
57894	PS TiAA, 15° P GH 2.5–4, SC / SCX / RS / RSX / RI*1 4.1 (solid abutment titanium Platform Switch)	76
57895	PS TiAA, 15° E GH 1–2, SC / SCX / RS / RSX / RI*1 4.1 (solid abutment titanium Platform Switch)	76
57896	PS TiAA, 15° E GH 2.5–4, SC / SCX / RS / RSX / RI*1 4.1 (solid abutment titanium Platform Switch)	76
57897	PS TiAA, 15° P GH 1–2, SC / SCX / RS / RSX / RI*1 4.5 (solid abutment titanium Platform Switch)	76
57898	PS TiAA, 15° P GH 2.5–4, SC / SCX / RS / RSX / RI*1 4.5 (solid abutment titanium Platform Switch)	76
57899	PS TiAA, 15° E GH 1–2, SC / SCX / RS / RSX / RI*1 4.5 (solid abutment titanium Platform Switch)	76
57900	PS TiAA, 15° E GH 2.5–4, SC / SCX / RS / RSX / RI*1 4.5 (solid abutment titanium Platform Switch)	76
57905	PS TiAA, 15° P GH 1–2, SC / SCX / RS / RSX / RI*1 5.5 (solid abutment titanium Platform Switch)	76
57906	PS TiAA, 15° P GH 2.5–4, SC / SCX / RS / RSX / RI*1 5.5 (solid abutment titanium Platform Switch)	76
57907	PS TiAA, 15° E GH 1–2, SC / SCX / RS / RSX / RI*1 5.5 (solid abutment titanium Platform Switch)	76
57908	PS TiAA, 15° E GH 2.5–4, SC / SCX / RS / RSX / RI*1 5.5 (solid abutment titanium Platform Switch)	76
57909	PS TiA, 20° P GH 1–2, SC / SCX / RS / RSX / RI*1 3.25–3.75 (solid abutment titanium Platform Switch)	77

Note: For manufacturer's information on trademarks, see page 122.

*1 New version of the BEGO Semados® RI implants, with Platform Switch Design

REF	Article	Page
57910	PS TiAA, 20° P GH 2.5–4, SC / SCX / RS / RSX / RI*1 3.25–3.75 (solid abutment titanium Platform Switch)	77
57911	PS TiAA, 20° E GH 1–2, SC / SCX / RS / RSX / RI*1 3.25–3.75 (solid abutment titanium Platform Switch)	77
57912	PS TiAA, 20° E GH 2.5–4, SC / SCX / RS / RSX / RI*1 3.25–3.75 (solid abutment titanium Platform Switch)	77
57913	PS TiAA, 20° P GH 1–2, SC / SCX / RS / RSX / RI*1 4.1 (solid abutment titanium Platform Switch)	77
57914	PS TiAA, 20° P GH 2.5–4, SC / SCX / RS / RSX / RI*1 4.1 (solid abutment titanium Platform Switch)	77
57915	PS TiAA, 20° E GH 1–2, SC / SCX / RS / RSX / RI*1 4.1 (solid abutment titanium Platform Switch)	77
57916	PS TiAA, 20° E GH 2.5–4, SC / SCX / RS / RSX / RI*1 4.1 (solid abutment titanium Platform Switch)	77
57917	PS TiAA, 20° P GH 1–2, SC / SCX / RS / RSX / RI*1 4.5 (solid abutment titanium Platform Switch)	77
57918	PS TiAA, 20° P GH 2.5–4, SC / SCX / RS / RSX / RI*1 4.5 (solid abutment titanium Platform Switch)	77
57919	PS TiAA, 20° E GH 1–2, SC / SCX / RS / RSX / RI*1 4.5 (solid abutment titanium Platform Switch)	77
57920	PS TiAA, 20° E GH 2.5–4, SC / SCX / RS / RSX / RI*1 4.5 (solid abutment titanium Platform Switch)	77
57921	PS TiAA, 20° P GH 1–2, SC / SCX / RS / RSX / RI*1 5.5 (solid abutment titanium Platform Switch)	77
57922	PS TiAA, 20° P GH 2.5–4, SC / SCX / RS / RSX / RI*1 5.5 (solid abutment titanium Platform Switch)	77
57923	PS TiAA, 20° E GH 1–2, SC / SCX / RS / RSX / RI*1 5.5 (solid abutment titanium Platform Switch)	77
57924	PS TiAA, 20° E GH 2.5–4, SC / SCX / RS / RSX / RI*1 5.5 (solid abutment titanium Platform Switch)	77
57926	Depth drill 2.5 short, RS / RSX-Line	49
57927	Depth drill 2.5 long, RS / RSX-Line	49

REF	Article	Page
57928	Depth drill short, RS / RSX 3.0	50
57929	Depth drill long, RS / RSX 3.0	50
57930	Depth drill short, RS / RSX 3.75	50
57931	Depth drill long, RS / RSX 3.75	50
57932	Depth drill short, RS / RSX 4.1	50
57933	Depth drill long, RS / RSX 4.1	50
57934	Depth drill short, RS / RSX 4.5	50
57935	Depth drill long, RS / RSX 4.5	50
57936	Depth drill short, RS / RSX 5.5	50
57937	Countersink, RS/R SX 3.0	50
57938	Countersink, RS/R SX 3.75	50
57939	Countersink, RS/R SX 4.1	50
57940	Countersink, RS/R SX 4.5	50
57941	Countersink, RS/R SX 5.5	50
57943	Screw tapper, RS/R SX 3.0	50
57944	Screw tapper, RS/R SX 3.75	50
57945	Screw tapper, RS/R SX 4.1	50
57946	Screw tapper, RS/R SX 4.5	50
57947	Screw tapper, RS/R SX 5.5	50
57948	Drill module, RS / RSX 5.5	49
57949	BEGO Semados® RS/R SX-Line tray ^{Plus}	49
57950	Implant cover screw, RS / RSX 3.0	28
57951	Implant cover screw, RS / RSX 3.75	28
57952	Implant cover screw, RS / RSX 4.1	28
57953	Implant cover screw, RS / RSX 4.5	28
57954	Implant cover screw, RS / RSX 5.5	28
57955	Depth gauge, RS/R SX-Line	58
57956	Paralleling post, RS/R SX-Line	57
57959	X-ray template, RS / RSX implants	16
57962	BEGO Semados® implant, RS 3.0 L10	22
57963	BEGO Semados® implant, RS 3.0 L11.5	22
57964	BEGO Semados® implant, RS 3.0 L13	22
57965	BEGO Semados® implant, RS 3.0 L15	22
57966	BEGO Semados® implant, RS 3.75 L8.5	22
57967	BEGO Semados® implant, RS 3.75 L10	22
57968	BEGO Semados® implant, RS 3.75 L11.5	22
57969	BEGO Semados® implant, RS 3.75 L13	22
57970	BEGO Semados® implant, RS 3.75 L15	22
57971	BEGO Semados® implant, RS 4.1 L7	22
57972	BEGO Semados® implant, RS 4.1 L8.5	22
57973	BEGO Semados® implant, RS 4.1 L10	22
57974	BEGO Semados® implant, RS 4.1 L11.5	22
57975	BEGO Semados® implant, RS 4.1 L13	22
57976	BEGO Semados® implant, RS 4.1 L15	22
57977	BEGO Semados® implant, RS 4.5 L7	22
57978	BEGO Semados® implant, RS 4.5 L8.5	22
57979	BEGO Semados® implant, RS 4.5 L10	22

REF	Article	Page
57980	BEGO Semados® implant, RS 4.5 L11.5	22
57981	BEGO Semados® implant, RS 4.5 L13	22
57982	BEGO Semados® implant, RS 4.5 L15	22
57983	BEGO Semados® implant, RS 5.5 L7	22
57984	BEGO Semados® implant, RS 5.5 L8.5	22
57985	BEGO Semados® implant, RS 5.5 L10	22
57986	BEGO Semados® implant, RS 5.5 L11.5	22
57987	BEGO Semados® implant, RS 5.5 L13	22
57988	TiBA Mini 2.7–3.1 (bar abutment titanium)	94
57989	TiA, Mini 2.9–3.1 (solid abutment titanium)	93
57993	PS UNI PScrew (prosthesis screw)	90
57994	PS UNI TScrew (technician screw)	89
57995	DD, Mini 2.7 (depth drill)	55
57996	DD, Mini 3.1 (depth drill)	55
57997	DD, Mini 2.9 (depth drill)	55
58051	BEGO Guide CS, (3), RS/RXS 3.0 (counter-sink for guided surgery)	42
58052	BEGO Guide CS, (4), RS/RXS 3.75 (countersink for guided surgery)	42
58053	BEGO Guide CS, (5), RS/RXS 4.1 (countersink for guided surgery)	42
58054	BEGO Guide CS, (6), RS/RXS 4.5 (countersink for guided surgery)	42
58055	BEGO Guide ST, (3), RS/RXS 3.0 (screw tapper for guided surgery)	43
58056	BEGO Guide ST, (4), RS/RXS 3.75 (screw tapper for guided surgery)	43
58057	BEGO Guide ST, (5), RS/RXS 4.1 (screw tapper for guided surgery)	43
58058	BEGO Guide ST, (6), RS/RXS 4.5 (screw tapper for guided surgery)	43
58059	BEGO Guide Conn, with contra-angle connection, Ø4.2 (AX), RS/RXS-Line (connector for guided surgery)	43
58060	BEGO Guide Conn, with contra-angle connection, Ø4.2 (AY), RS/RXS-Line (connector for guided surgery)	43
58061	BEGO Guide Conn, with contra-angle connection, Ø4.2 (AZ), RS/RXS-Line (connector for guided surgery)	43
58062	BEGO Guide Conn, with contra-angle connection, Ø4.7 (BX), RS/RXS-Line (connector for guided surgery)	43
58063	BEGO Guide Conn, with contra-angle connection, Ø4.7 (BY), RS/RXS-Line (connector for guided surgery)	43

REF	Article	Page
58064	BEGO Guide Conn, with contra-angle connection, Ø4.7 (BZ), RS/RXS-Line (connector for guided surgery)	43
58065	BEGO Guide Conn, with ratchet connection, Ø4.2 (AX), RS/RXS-Line (connector for guided surgery)	43
58066	BEGO Guide Conn, with ratchet connection, Ø4.2 (AY), RS/RXS-Line (connector for guided surgery)	43
58067	BEGO Guide Conn, with ratchet connection, Ø4.2 (AZ), RS/RXS-Line (connector for guided surgery)	43
58068	BEGO Guide Conn, with ratchet connection, Ø4.7 (BX), RS/RXS-Line (connector for guided surgery)	43
58069	BEGO Guide Conn, with ratchet connection, Ø4.7 (BY), RS/RXS-Line (connector for guided surgery)	43
58070	BEGO Guide Conn, with ratchet connection, Ø4.7 (BZ), RS/RXS-Line (connector for guided surgery)	43
58071	BEGO Guide Tr, RS/RXS-Line (tray for guided surgery)	41
58072	PS PPA, SC/SCX/RS/RXS/RI*1 3.25–3.75 (provisional abutment Platform Switch)	74
58073	PS PPA, SC / SCX / RS/RXS/ RI*1 4.1 (provisional abutment Platform Switch)	74
58074	PS PPA, SC / SCX / RS/RXS/ RI*1 4.5 (provisional abutment Platform Switch)	74
58075	PS PPA, SC / SCX / RS/RXS/ RI*1 5.5 (provisional abutment Platform Switch)	74
58076	PS ITA, SC/SCX/RS/RXS/RI*1 3.25–3.75 (provisional abutment Platform Switch)	74
58077	PS ITA, SC / SCX / RS/RXS/ RI*1 4.1 (provisional abutment Platform Switch)	74
58078	PS ITA, SC / SCX / RS/RXS/ RI*1 4.5 (provisional abutment Platform Switch)	74
58080	PS CA, SC/SCX/RS/RXS/RI*1 3.25–3.75 (ceramic abutment Platform Switch)	75
58081	PS CA, SC/SCX/RS/RXS/RI*1 4.1 (ceramic abutment Platform Switch)	75
58082	PS CA, SC/SCX/RS/RXS/RI*1 4.5 (ceramic abutment Platform Switch)	75
58083	PS CA, SC/SCX/RS/RXS/RI*1 5.5 (ceramic abutment Platform Switch)	75
58084	PS CATi, SC/SCX/RS/RXS/RI*1 3.25–3.75 (ceramic abutment Platform Switch)	75

Note: For manufacturer's information on trademarks, see page 122.

*1 New version of the BEGO Semados® RI implants, with Platform Switch Design

REF	Article	Page
58085	PS CATi, SC/SCX/RS/R SX/RI*1 4.1 (ceramic abutment Platform Switch)	75
58086	PS CATi, SC/SCX/RS/R SX/RI*1 4.5 (ceramic abutment Platform Switch)	75
58087	PS CATi, SC/SCX/RS/R SX/RI*1 5.5 (ceramic abutment Platform Switch)	75
58088	PS TiA, conical, SC / SCX / RS / RSX / RI*1 3.25–3.75 (solid abutment titanium Platform Switch)	75
58089	PS TiA, conical, SC / SCX / RS / RSX / RI*1 4.1 (solid abutment titanium Platform Switch)	75
58090	PS TiA, conical, SC / SCX / RS / RSX / RI*1 4.5 (solid abutment titanium Platform Switch)	75
58091	PS TiA, conical, SC / SCX / RS / RSX / RI*1 5.5 (solid abutment titanium Platform Switch)	75
58092	PS GCO, SC/SCX/RS/R SX/RI*1 3.25–3.75 (gold cast-on abutment Platform Switch)	79
58093	PS GCO, SC/SCX/RS/R SX/RI*1 4.1 (gold cast-on abutment Platform Switch)	79
58094	PS GCO, SC/SCX/RS/R SX/RI*1 4.5 (gold cast-on abutment Platform Switch)	79
58095	PS GCO, SC/SCX/RS/R SX/RI*1 5.5 (gold cast-on abutment Platform Switch)	79
58096	PS GCO NH, SC / SCX / RS/R SX/ RI*1 3.25–3.75 (gold cast-on abutment no Hex Platform Switch)	79
58097	PS GCO NH, SC / SCX / RS/R SX/ RI*1 4.1 (gold cast-on abutment no Hex Platform Switch)	79
58098	PS GCO NH, SC / SCX / RS/R SX/ RI*1 4.5 (gold cast-on abutment no Hex Platform Switch)	79
58099	PS GCO NH, SC / SCX / RS/R SX/ RI*1 5.5 (gold cast-on abutment no Hex Platform Switch)	79
58100	PS MultiPlus, 0° GH 1, SC/SCX/RS/R SX/RI*1 3.25–3.75 (MultiPlus abutment Platform Switch)	80
58101	PS MultiPlus, 0° GH 3, SC/SCX/RS/R SX/RI*1 3.25–3.75 (MultiPlus abutment Platform Switch)	79
58102	PS MultiPlus, 0° GH 1, SC/SCX/RS/R SX/RI*1 4.1 (MultiPlus abutment Platform Switch)	79
58103	PS MultiPlus, 0° GH 3, SC/SCX/RS/R SX/RI*1 4.1 (MultiPlus abutment Platform Switch)	79
58104	PS MultiPlus, 0° GH 1, SC/SCX/RS/R SX/RI*1 4.5 (MultiPlus abutment Platform Switch)	79

REF	Article	Page
58105	PS MultiPlus, 0° GH 3, SC/SCX/RS/R SX/RI*1 4.5 (MultiPlus abutment Platform Switch)	79
58108	PS MultiPlus, 20° GH 2.3–0.6, SC/SCX/RS/R SX/RI*1 3.25–3.75 (MultiPlus abutment Platform Switch)	81
58109	PS MultiPlus, 20° GH 4.0–2.3, SC/SCX/RS/R SX/RI*1 3.25–3.75 (MultiPlus abutment Platform Switch)	81
58110	PS MultiPlus, 20° GH 2.3–0.6, SC/SCX/RS/R SX/RI*1 4.1 (MultiPlus abutment Platform Switch)	81
58111	PS MultiPlus, 20° GH 4.0–2.3, SC/SCX/RS/R SX/RI*1 4.1 (MultiPlus abutment Platform Switch)	81
58112	PS MultiPlus, 20° GH 2.3–0.6, SC/SCX/RS/R SX/RI*1 4.5 (MultiPlus abutment Platform Switch)	81
58113	PS MultiPlus, 20° GH 4.0–2.3, SC/SCX/RS/R SX/RI*1 4.5 (MultiPlus abutment Platform Switch)	81
58116	PS MultiPlus, 30° GH 4.0–1.5, SC/SCX/RS/R SX/RI*1 3.25–3.75 (MultiPlus abutment Platform Switch)	81
58117	PS MultiPlus, 30° GH 4.0–1.5, SC/SCX/RS/R SX/RI*1 4.1 (MultiPlus abutment Platform Switch)	81
58118	PS MultiPlus, 30° GH 4.0–1.5, SC/SCX/RS/R SX/RI*1 4.5 (MultiPlus abutment Platform Switch)	81
58120	PS BA, GH 0, SC/SCX/RS/R SX/RI*1 3.25–3.75 (ball attachment abutment Platform Switch)	85
58121	PS BA, GH 3, SC/SCX/RS/R SX/RI*1 3.25–3.75 (ball attachment abutment Platform Switch)	85
58122	PS BA, GH 5, SC/SCX/RS/R SX/RI*1 3.25–3.75 (ball attachment abutment Platform Switch)	85
58123	PS BA, GH 0, SC/SCX/RS/R SX/RI*1 4.1 (ball attachment abutment Platform Switch)	85
58124	PS BA, GH 3, SC/SCX/RS/R SX/RI*1 4.1 (ball attachment abutment Platform Switch)	85
58125	PS BA, GH 5, SC/SCX/RS/R SX/RI*1 4.1 (ball attachment abutment Platform Switch)	85
58126	PS BA, GH 0, SC/SCX/RS/R SX/RI*1 4.5 (ball attachment abutment Platform Switch)	85

REF	Article	Page
58127	PS BA, GH 3, SC/SCX/RS/RXS/RI*1 4.5 (ball attachment abutment Platform Switch)	85
58128	PS BA, GH 5, SC/SCX/RS/RXS/RI*1 4.5 (ball attachment abutment Platform Switch)	85
58130	PS Easy-Con, L1, SC/SCX/RS/RXS/RI*1 3.25–3.75 (Easy-Con abutment Platform Switch)	86
58131	PS Easy-Con, L2, SC/SCX/RS/RXS/RI*1 3.25–3.75 (Easy-Con abutment Platform Switch)	86
58132	PS Easy-Con, L3, SC/SCX/RS/RXS/RI*1 3.25–3.75 (Easy-Con abutment Platform Switch)	86
58133	PS Easy-Con, L4, SC/SCX/RS/RXS/RI*1 3.25–3.75 (Easy-Con abutment Platform Switch)	86
58134	PS Easy-Con, L1, SC/SCX/RS/RXS/RI*1 4.1 (Easy-Con abutment Platform Switch)	86
58135	PS Easy-Con, L2, SC/SCX/RS/RXS/RI*1 4.1 (Easy-Con abutment Platform Switch)	86
58136	PS Easy-Con, L3, SC/SCX/RS/RXS/RI*1 4.1 (Easy-Con abutment Platform Switch)	86
58137	PS Easy-Con, L4, SC/SCX/RS/RXS/RI*1 4.1 (Easy-Con abutment Platform Switch)	86
58138	PS Easy-Con, L1, SC/SCX/RS/RXS/RI*1 4.5 (Easy-Con abutment Platform Switch)	86
58139	PS Easy-Con, L2, SC/SCX/RS/RXS/RI*1 4.5 (Easy-Con abutment Platform Switch)	86
58140	PS Easy-Con, L3, SC/SCX/RS/RXS/RI*1 4.5 (Easy-Con abutment Platform Switch)	86
58141	PS Easy-Con, L4, SC/SCX/RS/RXS/RI*1 4.5 (Easy-Con abutment Platform Switch)	86
58142	PS Easy-Con, L2, SC/SCX/RS/RXS/RI*1 5.5 (Easy-Con abutment Platform Switch)	86
58143	PS Easy-Con, L4, SC/SCX/RS/RXS/RI*1 5.5 (Easy-Con abutment Platform Switch)	86
58146	PS TPA, SC/SCX/RS/RXS/RI*1 3.25–3.75 (provisional abutment Platform Switch)	74
58147	PS TPA, SC / SCX / RS/RXS / RI*1 4.1 (provisional abutment Platform Switch)	74
58148	PS TPA, SC / SCX / RS/RXS / RI*1 4.5 (provisional abutment Platform Switch)	74
58150	PS HP, Ø4.5 L7, SC / SCX / RS/RXS / RI*1 3.25–3.75 (healing post Platform Switch)	28
58151	PS HP, Ø5.0 L7, SC / SCX / RS/RXS / RI*1 4.1 (healing post Platform Switch)	28
58152	PS HP, Ø5.5 L7, SC / SCX / RS/RXS / RI*1 4.5 (healing post Platform Switch)	28
58153	PS HP, Ø6.5 L7, SC / SCX / RS/RXS / RI*1 5.5 (healing post Platform Switch)	28

REF	Article	Page
58155	PS TiBA, SC/SCX/RS/RXS/RI*1 3.25–3.75 (bar abutment titanium Platform Switch)	88
58156	PS TiBA, SC/SCX/RS/RXS/RI*1 4.1 (bar abutment titanium Platform Switch)	88
58157	PS TiBA, SC/SCX/RS/RXS/RI*1 4.5 (bar abutment titanium Platform Switch)	88
58160	BEGO Semados® implant, SC 3.25 L8.5	18
58161	BEGO Semados® implant, SC 3.25 L10	18
58162	BEGO Semados® implant, SC 3.25 L11.5	18
58163	BEGO Semados® implant, SC 3.25 L13	18
58164	BEGO Semados® implant, SC 3.25 L15	18
58165	BEGO Semados® implant, SC 3.75 L8.5	18
58166	BEGO Semados® implant, SC 3.75 L10	18
58167	BEGO Semados® implant, SC 3.75 L11.5	18
58168	BEGO Semados® implant, SC 3.75 L13	18
58169	BEGO Semados® implant, SC 3.75 L15	18
58170	BEGO Semados® implant, SC 4.1 L7	18
58171	BEGO Semados® implant, SC 4.1 L8.5	18
58172	BEGO Semados® implant, SC 4.1 L10	18
58173	BEGO Semados® implant, SC 4.1 L11.5	18
58174	BEGO Semados® implant, SC 4.1 L13	18
58175	BEGO Semados® implant, SC 4.1 L15	18
58176	BEGO Semados® implant, SC 4.5 L7	18
58177	BEGO Semados® implant, SC 4.5 L8.5	18
58178	BEGO Semados® implant, SC 4.5 L10	18
58179	BEGO Semados® implant, SC 4.5 L11.5	18
58180	BEGO Semados® implant, SC 4.5 L13	18
58181	BEGO Semados® implant, SC 4.5 L15	18
58182	BEGO Semados® implant, SC 5.5 L7	18
58183	BEGO Semados® implant, SC 5.5 L8.5	18
58184	BEGO Semados® implant, SC 5.5 L10	18
58185	BEGO Semados® implant, SC 5.5 L11.5	18
58186	BEGO Semados® implant, SC 5.5 L13	18
58190	CAD SP, RS / RSX 3.0 (scansupport)	68
58191	CAD SP, S/SC/SCX/RS/RXS/RI 3.25–3.75 (scansupport)	69, 103
58192	CAD SP, S/SC/SCX/RS/RXS/RI 4.1 (scansupport)	69, 103
58193	CAD SP, S/SC/SCX/RS/RXS/RI 4.5 (scansupport)	69, 103
58194	CAD SP, S/SC/SCX/RS/RXS/RI 5.5 (scansupport)	69, 103
58200	PS HPW, Ø5.5 L5, SC / SCX / RS/RXS / RI*1 3.25–3.75 (healing post Platform Switch)	29
58201	PS HPW, Ø5.5 L7, SC / SCX / RS/RXS / RI*1 3.25–3.75 (healing post Platform Switch)	29
58202	PS HPW, Ø6.0 L5, SC / SCX / RS/RXS / RI*1 4.1 (healing post Platform Switch)	29
58203	PS HPW, Ø6.0 L7, SC / SCX / RS/RXS / RI*1 4.1 (healing post Platform Switch)	29

Note: For manufacturer's information on trademarks, see page 122.

*1 New version of the BEGO Semados® RI implants, with Platform Switch Design

REF	Article	Page
58204	PS HPW, Ø6.5 L5, SC / SCX / RS/R SX / RI*1 4.5 (healing post Platform Switch)	29
58205	PS HPW, Ø6.5 L7, SC / SCX / RS/R SX / RI*1 4.5 (healing post Platform Switch)	29
58206	PS HPW, Ø7.0 L5, SC / SCX / RS/R SX / RI*1 5.5 (healing post Platform Switch)	29
58207	PS HPW, Ø7.0 L7, SC / SCX / RS/R SX / RI*1 5.5 (healing post Platform Switch)	29
58219	ST PMB, Ø16, S/RI 3.25–5.5 (CAD/CAM milling blank)	103
58226	PS GCO, Ø16, SC/SCX/RS/R SX/RI*1 3.25–5.5 (CAD/CAM milling blank Platform Switch)	70
58240	MultiPlus MC (MultiPlus Easy-Con abutment)	83, 113
58242	BEGO Semados® SCX implant large-scale model	120
58243	Maxilla demonstration model, SCX implants	121
58244	BEGO Semados® SC demo implants	121
58245	BEGO Semados® SCX demo implants	121
58246	X-ray template, SC / SCX implants	16
58247	PS AS (assortment set Platform Switch)	77
58250	PS CADP, RS / RSX 3.0 (CAD positioner Platform Switch)	68
58251	PS CADP, SC/SCX/RS/R SX/RI*1 3.25–3.75 (CAD positioner Platform Switch)	69
58252	PS CADP, SC/SCX/RS/R SX/RI*1 4.1 (CAD positioner Platform Switch)	69
58253	PS CADP, SC/SCX/RS/R SX/RI*1 4.5 (CAD positioner Platform Switch)	69
58254	PS CADP, SC/SCX/RS/R SX/RI*1 5.5 (CAD positioner Platform Switch)	69
58255	CADP MultiPlus (CAD positioner)	82, 112
58256	CADP, Mini-Line (CAD positioner)	92
58260	BEGO Semados® implant, SCX 3.25 L8.5	19
58261	BEGO Semados® implant, SCX 3.25 L10	19
58262	BEGO Semados® implant, SCX 3.25 L11.5	19
58263	BEGO Semados® implant, SCX 3.25 L13	19
58264	BEGO Semados® implant, SCX 3.25 L15	19
58265	BEGO Semados® implant, SCX 3.75 L8.5	19
58266	BEGO Semados® implant, SCX 3.75 L10	19
58267	BEGO Semados® implant, SCX 3.75 L11.5	19
58268	BEGO Semados® implant, SCX 3.75 L13	19
58269	BEGO Semados® implant, SCX 3.75 L15	19
58270	BEGO Semados® implant, SCX 4.1 L7	19
58271	BEGO Semados® implant, SCX 4.1 L8.5	19
58272	BEGO Semados® implant, SCX 4.1 L10	19
58273	BEGO Semados® implant, SCX 4.1 L11.5	19
58274	BEGO Semados® implant, SCX 4.1 L13	19

REF	Article	Page
58275	BEGO Semados® implant, SCX 4.1 L15	19
58276	BEGO Semados® implant, SCX 4.5 L7	19
58277	BEGO Semados® implant, SCX 4.5 L8.5	19
58278	BEGO Semados® implant, SCX 4.5 L10	19
58279	BEGO Semados® implant, SCX 4.5 L11.5	19
58280	BEGO Semados® implant, SCX 4.5 L13	19
58281	BEGO Semados® implant, SCX 4.5 L15	19
58282	BEGO Semados® implant, SCX 5.5 L7	19
58283	BEGO Semados® implant, SCX 5.5 L8.5	19
58284	BEGO Semados® implant, SCX 5.5 L10	19
58285	BEGO Semados® implant, SCX 5.5 L11.5	19
58286	BEGO Semados® implant, SCX 5.5 L13	19
58290	Implant cover screw, SC / SCX 3.25	28
58297	PS OCP, GH 1, SC/SCX/RS/R SX/RI*1 3.25–3.75 (restoration set Platform Switch)	71
58298	PS OCP, GH 1, SC/SCX/RS/R SX/RI*1 4.1 (restoration set Platform Switch)	71
58299	PS OCP, GH 1, SC/SCX/RS/R SX/RI*1 4.5 (restoration set Platform Switch)	71
58300	PS OCP, GH 3, SC/SCX/RS/R SX/RI*1 3.25–3.75 (restoration set Platform Switch)	71
58301	PS OCP, GH 3, SC/SCX/RS/R SX/RI*1 4.1 (restoration set Platform Switch)	71
58302	PS OCP, GH 3, SC/SCX/RS/R SX/RI*1 4.5 (restoration set Platform Switch)	71
58303	LCC (laboratory caps crown)	71
58304	LCB (laboratory caps bridge)	71
58305	OCP A (implant analog)	71
58315	PS IMPA, SC / SCX 3.25 (implant analog Platform Switch)	72
58316	PS CTI, SC/SCX 3.25 (impression set (closed) Platform Switch)	72
58317	PS CTI, SC/SCX 3.25 (impression set (open) Platform Switch)	72
58319	ST PMB, Ø11.5, S/RI 3.25–5.5 (CAD/CAM milling blank)	103
58322	BEGO Semados® RI*1 implant large-scale model	120
58326	PS PMB, Ø11.5, SC/SCX/RS/R SX/RI*1 3.25–5.5 (CAD/CAM milling blank Platform Switch)	70
58345	BEGO Semados® RI*1 demo implant	121

A		
Acrylic block PS-Line (large-scale model, scale 2:1)	120	
B		
Ball attachment impression set Dalbo®-PLUS	85, 96, 115	
Ball attachment Mini	96	
BeCe® Sub-Tec ceramic abutments (S / RI implants)	106	
BeCe® Sub-Tec ^{Plus} ceramic abutments (S / RI implants)	106	
BEGO Collagen Fleece	10	
BEGO Collagen Membrane	10	
BEGO Guide – pilot drill	44	
BEGO Guide centre drill (S / RS / RSX-Line)	39, 42	
BEGO Guide Conn, with contra-angle connection (connector for guided surgery, RS / RSX-Line)	43	
BEGO Guide Conn, with ratchet connection (connector for guided surgery, RS / RSX-Line)	43	
BEGO Guide connector (S-Line)	40	
BEGO Guide countersink (S-Line)	39	
BEGO Guide CS (Countersink for guided surgery, RS / RSX-Line)	42	
BEGO Guide DD (depth drill for guided surgery, RS / RSX-Line)	42	
BEGO Guide depth drill (S-Line)	39	
BEGO Guide depth stop ring connector (S / RS / RSX-Line)	40, 43	
BEGO Guide DS (drill sleeves for guided surgery)	44	
BEGO Guide master sleeves (S / RS / RSX-Line)	38, 41	
BEGO Guide PD (pilot drill for guided surgery, RS / RSX-Line)	42	
BEGO Guide pilot drill (S-Line)	39	
BEGO Guide ratchet adapter for connector (S-Line)	40	
BEGO Guide screw tapper (S-Line)	40	
BEGO Guide S-Line tray	38	
BEGO Guide Sp (reduction sleeve for guided surgery, RS / RSX-Line)	41	
BEGO Guide spoons (S-Line)	38	
BEGO Guide ST (screw tapper for guided surgery, RS / RSX-Line)	43	
BEGO Guide tissue punches (S / RS / RSX-Line)	38, 41	
BEGO Guide Tr (tray for guided surgery, RS / RSX-Line)	41	
BEGO OSS	10	
BEGO OSS S	10	
BEGO Semados® Mini demo implants	121	
BEGO Semados® Mini implant large-scale model	120	
BEGO Semados® Mini implants	32	
BEGO Semados® PI tray	34	
BEGO Semados® Provisional Implant (PI)	34	
BEGO Semados® ratchet adapter	58, 60	
BEGO Semados® RI*1 demo implant	121	
BEGO Semados® RI*1 implant large-scale model	120	
BEGO Semados® RI*1 implants	26	
BEGO Semados® RI-Line tray	52	
BEGO Semados® RS demo implants	121	
BEGO Semados® RS implants	22	
BEGO Semados® RS / RSX-Line tray	49	
BEGO Semados® RSX demo implants	121	
BEGO Semados® RSX demo implants Ø 3.0	121	
BEGO Semados® RSX implant large-scale model	120	
BEGO Semados® RSX implants	23	
BEGO Semados® SC demo implants	121	
BEGO Semados® SC implants	18	
BEGO Semados® SCX demo implants	121	
BEGO Semados® SCX implant large-scale model	121	
BEGO Semados® SCX implants	19	
BEGO Semados® S-Line tray ^{Plus}	46	
Bone profiler (S / RI implants)	56	
C		
CAD SP (scansupport, RS / RSX 3.0)	68	
CAD SP (scansupport, S / SC / SCX / RS / RSX / RI)	69, 103	
CADP (CAD positioner, Mini-Line)	92	
CADP Multi ^{Plus} (CAD positioner)	82, 112	
Countersink (RI-Line)	53	
Countersink (RS / RSX-Line)	50	
Countersink (S-Line)	47	
D		
Dalbo-PLUS activator / deactivator	85, 96, 115	
DD (depth drill, Mini-Line)	55	
DD D1 (depth drill, RS / RSX-Line)	50	
Depth drill (RI-Line)	53	
Depth drill (RS / RSX-Line)	50	
Depth drill (S-Line)	47	
Depth drill 2.5 (RS / RSX-Line)	49	
Depth drill 2.5 (S-Line)	46	
Depth drill 3.2 (RI-Line)	52	
Depth gauge	58	
DOLDER® bar joint attachment 3.0 – titanium	88, 94	
Drill extension one-part (without internal cooling)	57	
Drill module (RI 5.5)	52	
Drill module (RS / RSX 5.5)	49	
Drill module (S / SC / SCX 5.5)	46	
Drill sleeves (1.6 / 2.5 / 3.2 mm)	16	
Drill stop tray ^{Plus} (RI-Line)	54	
Drill stop tray ^{Plus} (RS / RSX-Line)	51	
Drill stop tray ^{Plus} (S-Line)	48	
Drill stops (RI-Line)	54	
Drill stops (RS / RSX-Line)	51	
Drill stops (S-Line)	48	

Note: For manufacturer's information on trademarks, see page 122.

*1 New version of the BEGO Semados® RI implants, with Platform Switch Design

E		
Easy-Con analog	86, 94, 116	
Easy-Con fabrication insert	87, 95, 117	
Easy-Con impression coping	86, 94, 116	
Easy-Con instrument	87, 95, 117	
Easy-Con laboratory set	87, 95, 117	
Easy-Con Mini	94	
Easy-Con retention inserts	87, 95, 117	
F		
Female parts Dalbo-PLUS	85, 96, 115	
Fibreglass pen	58	
G		
Gap-cutter disc (Mini-Line)	55	
Gap-cutter drill (Mini-Line)	55	
Gold cast-on Mini	93	
Guiding wrench	57	
H		
Healing posts (S / RI implants)	100	
Healing posts individual, Ø 7 (S / RS / RSX / RI-Line)	29, 100	
Healing posts Mini	32	
Healing posts, conical (S / RI implants)	100	
Hexagon screwdriver 1.25 mm, contra-angle	60	
Hexagon screwdriver 1.25 mm, with ratchet connection	60	
I		
IDC (implant adjustment instrument)	57	
Implant cover screw Mini	32	
Implant cover screws (S / RI implants)	100	
Implant cover screws (S / SC / SCX / RS / RSX / RI*1)	28	
Initial drill (Mini-Line)	55	
Insertion instrument MultiPlus abutment O°	80, 110	
Insertion tool for ball attachment	85, 96, 115	
Insertion tool for implants, with contra-angle connection	57	
Insertion tool for implants, with ratchet connection	57	
Insertion tool Locator	86, 94, 116	
Internal reamer for gold cast-on abutment	79, 109	
Internal reamer for gold cast-on Mini	93	
L		
Large-scale models – demonstration suitcase	120	
LCB (laboratory caps bridge)	71	
LCC (laboratory caps crown)	71	
M		
Maxilla demonstration model	121	
Measuring spheres	16	
Mini- / OsseoPlus tray	55	
Model implant Mini	92	
Model implants (S / RI implants)	104	
MultiPlus alignment aids	80, 110	
MultiPlus bone shaper	80, 110	
MultiPlus closed tray impression	82, 112	
MultiPlus gold cast-on	84, 114	
MultiPlus healing cap	81, 111	
MultiPlus healing cap Mushroom	81, 111	
MultiPlus implant analog	82, 112	
MultiPlus insertion splint	80, 110	
MultiPlus MC (MultiPlus Easy-Con abutment)	83, 112	
MultiPlus open tray impression	82, 112	
MultiPlus protection analog	83, 112	
MultiPlus titanium abutment	83, 112	
MultiPlus Universal	84, 114	
O		
OCP A (implant analog)	71	
Open tray impression Mini	92	
P		
Paralleling post	57	
PI bending instrument	35	
PI depth drill	35	
PI implant analog	34	
PI multifunctional cap	34	
PI paralleling post	35	
PI protection cap	34	
PI ratchet	35	
PI removal tool	35	
PI stabiliser	35	
Pilot drill (S-Line)	46	
Pilot marker (RI-Line)	52	
Pilot marker (RS / RSX-Line)	49	
Pilot marker (S-Line)	46	
Prosthesis screw for ceramic abutment	90, 118	
Prosthesis screw Hex 1.25 mm	90, 118	
Prosthesis screw Mini	97	
Prosthesis screw Mini, conical	97	
Prosthesis screw MultiPlus (M1.8)	90, 118	
Prosthesis screw Sub-TecPlus	90, 118	
Prosthesis screws Sub-TecPlus Universal	118	
Prosthetic kit	60	
PS AS (assortment set Platform Switch, SC / SCX / RS / RSX / RI*1)	77	
PS BA (ball attachment abutment Platform Switch, SC / SCX / RS / RSX / RI*1)	85	
PS CA (ceramic abutment Platform Switch) SC / SCX / RS / RSX / RI*1	75	
PS CADP (CAD positioner Platform Switch, RS / RSX Ø 3.0)	68	
PS CADP (CAD positioner Platform Switch, SC / SCX / RS / RSX / RI*1)	69	
PS CATi (ceramic abutment Platform Switch)	75	

PS CTI (impression set (closed) Platform Switch) SC / SCX / RS / RSX / RI* ¹	72
PS Easy-Con (Easy-Con abutment Platform Switch, SC / SCX / RS / RSX / RI* ¹)	86
PS GCO (gold cast-on abutment Platform Switch, SC / SCX / RS / RSX / RI* ¹)	79
PS GCO NH (gold cast-on abutment no Hex Platform Switch, SC / SCX / RS / RSX / RI* ¹)	79
PS HP (healing posts Platform Switch, SC / SCX / RS / RSX / RI* ¹)	28
PS HPW (healing posts Platform Switch, SC / SCX / RS / RSX / RI* ¹)	29
PS IMPA (implant analog Platform Switch, SC / SCX / RS / RSX / RI* ¹)	72
PS ITA (provisional abutment Platform Switch, SC / SCX / RS / RSX / RI* ¹)	74
PS ITA (provisional abutment Platform Switch, RS / RSX 3.0)	73
PS Multi ^{Plus} (Multi ^{Plus} abutment Platform Switch) SC / SCX / RS / RSX / RI* ¹	80, 81
PS OCP (restoration set Platform Switch, SC / SCX / RS / RSX / RI* ¹)	71
PS OTI (impression set (open) Platform Switch, SC / SCX / RS / RSX / RI* ¹)	72
PS PMB (CAD / CAM milling blank Platform Switch, SC / SCX / RS / RSX / RI* ¹)	70
PS PPA (provisional abutment Platform Switch, SC / SCX / RS / RSX / RI* ¹)	74
PS TiA (solid abutment titanium Platform Switch, RS / RSX 3.0)	73
PS TiA (solid abutment titanium Platform Switch, SC / SCX / RS / RSX / RI* ¹)	75, 76
PS TiAA (solid abutment titanium Platform Switch, RS / RSX-Line 3.0)	73
PS TiAA (solid abutment titanium Platform Switch), SC / SCX / RS / RSX / RI* ¹	76, 77
PS TiB (adhesive abutment Platform Switch) SC / SCX / RS / RSX / RI* ¹	69
PS TiB (adhesive abutment Platform Switch, RS / RSX 3.0)	68
PS TiB NH (adhesive abutment no Hex Platform Switch, SC / SCX / RS / RSX / RI* ¹)	70
PS TiBA (bar abutment titanium Platform Switch) SC / SCX / RS / RSX / RI* ¹	88
PS TPA (provisional abutment Platform Switch, SC / SCX / RS / RSX / RI* ¹)	74

PS TTiA (provisional abutment Platform Switch, SC / SCX / RS / RSX / RI* ¹)	74
PS TTiA NH (provisional abutment no Hex Platform Switch, SC / SCX / RS / RSX / RI* ¹)	74
PS UNI (Universal abutment Platform Switch, SC / SCX / RS / RSX / RI* ¹)	78
PS UNI NH (Universal abutment no Hex Platform Switch, SC / SCX / RS / RSX / RI* ¹)	78
PS UNI PScrew (prosthesis screw)	90
PS UNI TScrew (technician screw)	89
PScrew (prosthesis screw)	90
R	
Radiograph templates	16
Ratchet / torque wrench	58, 60
Reamers Multi ^{Plus}	84, 114
Reamers Universal	78, 108
Replacement brush for the fibreglass pen	58
Retention insert Dalbo-PLUS	85, 96, 115
S	
Screw tapper (RI-Line)	53
Screw tapper (RS / RSX-Line)	50
Screw tapper (S-Line)	47
Secondary screw Multi ^{Plus} (M1.4)	90, 118
Slot screwdriver short, with ratchet connection	60
ST PMB (CAD / CAM milling blank, S / RI implants)	90
Sub-Dent closed tray impression (S / RI implants)	104
Sub-Dent open tray impression (S / RI implants)	104
Sub-Tec ball attachment (S / RI implants)	115
Sub-Tec CAD positioner (S / RI implants)	102
Sub-Tec CAD / CAM TiBase L (S / RI implants)	103
Sub-Tec CAD / CAM titanium adhesive abutment (S / RI implants)	102
Sub-Tec CAD / CAM titanium adhesive abutment no Hex (S / RI implants)	102
Sub-Tec Easy-Con abutment (S / RI implants)	116
Sub-Tec gold cast-on (S / RI implants)	109
Sub-Tec gold cast-on no Hex (S / RI implants)	109
Sub-Tec Multi ^{Plus} abutment (S / RI implants)	110, 111
Sub-Tec provisional abutment Ø 7 (S / RI implants)	105
Sub-Tec provisional PEEK abutment (S / RI implants)	105
Sub-Tec provisional titanium abutment (S / RI implants)	105
Sub-Tec provisional titanium abutment no Hex (S / RI implants)	105
Sub-Tec ^{Plus} titanium abutment (S / RI implants)	106
Sub-Tec ^{Plus} titanium angulated abutment (S / RI implants)	107
Sub-Tec Universal (S / RI implants)	108
Sub-Tec Universal no Hex (S / RI implants)	108

Note: For manufacturer's information on trademarks, see page 122.

*¹ New version of the BEGO Semados® RI implants, with Platform Switch Design

T	
Technician screw L9	89
Technician screw Mini	97
Technician screw Mini, conical	97
Technician screw Multi ^{Plus} (M1.4)	89
Technician screw Sub-Tec ^{Plus}	89
Threadformer (Mini-Line)	55
Threadformer (RI-Line)	53
TiA (solid abutment titanium, Mini-Line)	93
TiBA (bar abutment Titan, Mini-Line)	94
Tissue punches (S / SC / SCX / RS / RSX / RI)	46, 49, 52
TJL (training case, mandible)	122
TJU (training case, maxilla)	122
Trepan drill	56
TScrew (technician screw)	89

www.bego.com



Customer number

BEGO Implant Systems GmbH & Co. KG
Wilhelm-Herbst-Str. 1 · 28359 Bremen, Germany
Tel. +49 421 2028-246 · Fax +49 421 2028-265
email info@bego-implantology.com · www.bego.com